

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
 Data File : VV023680.D
 Acq On : 23 Nov 2021 18:54
 Operator : SY/MD
 Sample : M4723-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G25

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	30	rVB2	21273	21580	4.51%	0.552%
2	1.307	75	83	99	rVB	91944	96367	20.14%	2.467%
3	1.568	155	164	176	rBV	68722	80010	16.73%	2.048%
4	2.111	320	333	348	rBV	131183	192189	40.17%	4.920%
5	3.896	876	888	918	rBV2	36999	136953	28.63%	3.506%
6	4.349	1013	1029	1049	rBV2	86892	214851	44.91%	5.500%
7	5.050	1229	1247	1275	rBV2	186194	478382	100.00%	12.247%
8	5.616	1412	1423	1450	rBV2	149664	307850	64.35%	7.881%
9	6.069	1551	1564	1594	rBV	107139	223864	46.80%	5.731%
10	6.989	1839	1850	1869	rBV	50703	98351	20.56%	2.518%
11	7.317	1938	1952	1971	rBV	227055	398741	83.35%	10.208%
12	7.400	1972	1978	1986	rVB4	4874	8410	1.76%	0.215%
13	7.625	2038	2048	2063	rBV2	30124	54964	11.49%	1.407%
14	8.092	2181	2193	2222	rBV2	180893	366034	76.52%	9.371%
15	8.854	2418	2430	2448	rBV	231490	385403	80.56%	9.867%
16	10.217	2843	2854	2878	rBV	73859	115849	24.22%	2.966%
17	10.384	2893	2906	2917	rVB2	7169	10729	2.24%	0.275%
18	11.249	3164	3175	3195	rBV	216495	342567	71.61%	8.770%
19	11.532	3255	3263	3279	rBV2	13317	24127	5.04%	0.618%
20	11.625	3279	3292	3315	rVB	217804	348811	72.91%	8.930%




Sum of corrected areas: 3906032

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023680.D
Acq On : 23 Nov 2021 18:54
Operator : SY/MD
Sample : M4723-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

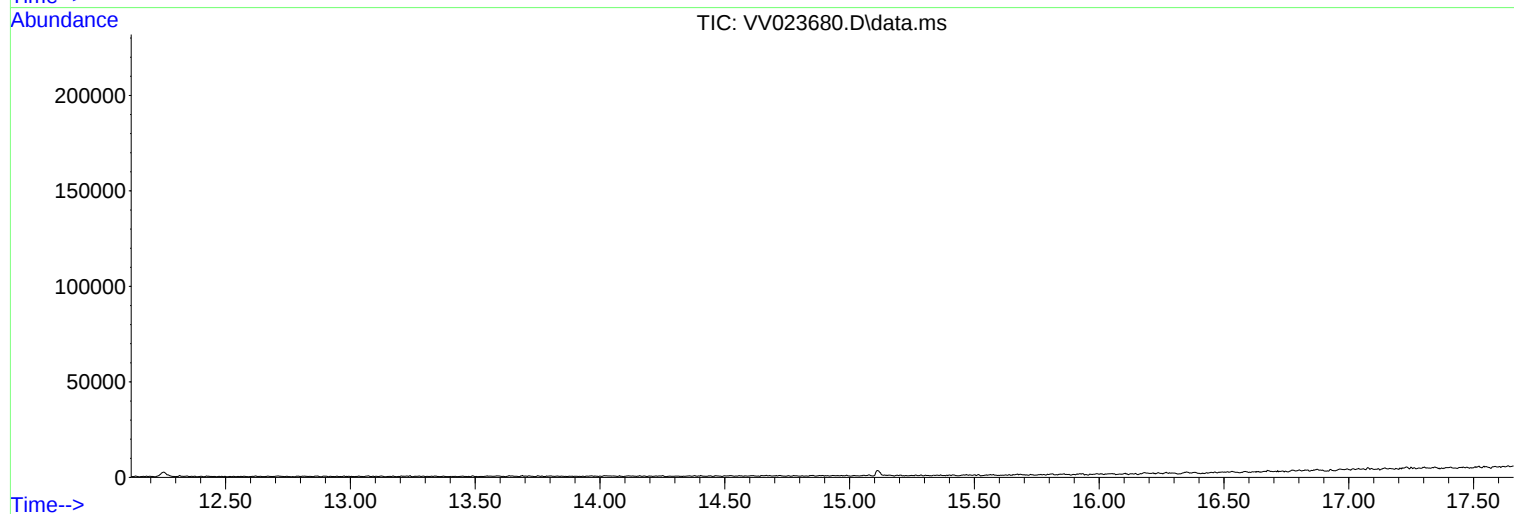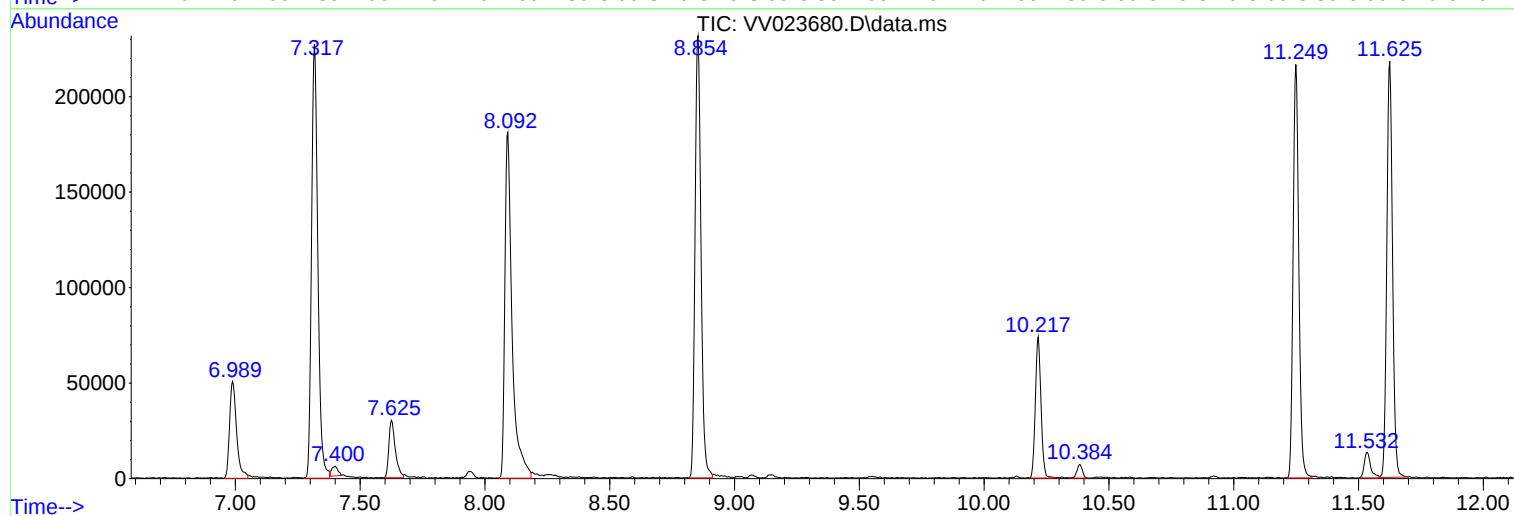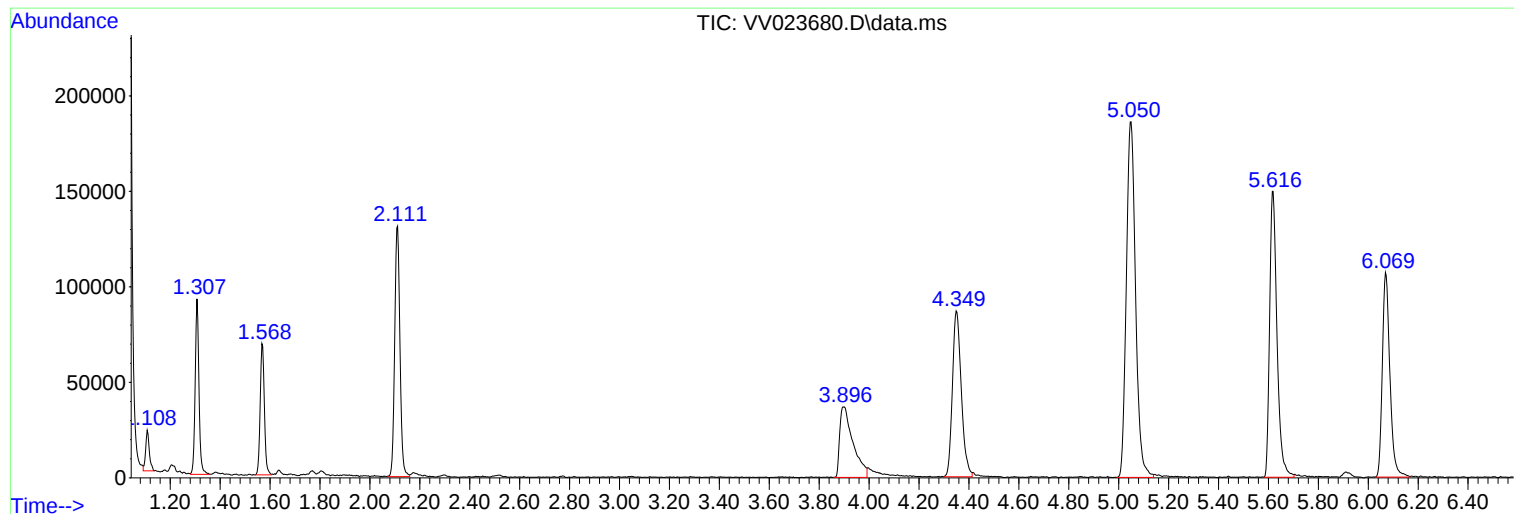

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023680.D
Acq On : 23 Nov 2021 18:54
Operator : SY/MD
Sample : M4723-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023680.D
Acq On : 23 Nov 2021 18:54
Operator : SY/MD
Sample : M4723-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
