
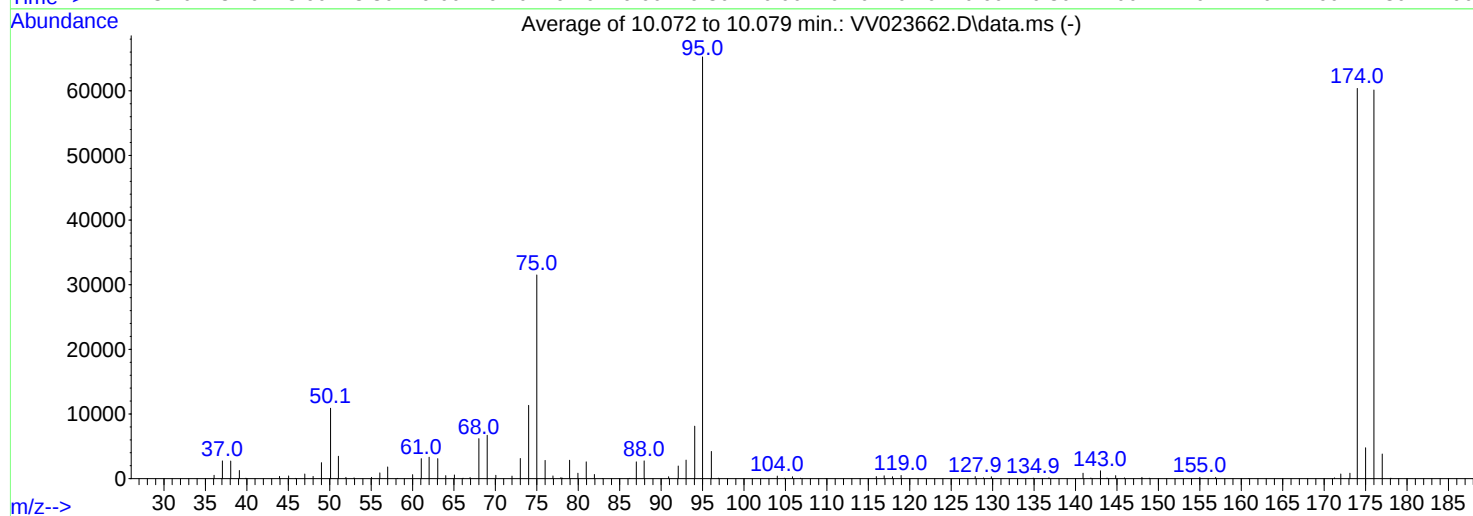


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
 Data File : VV023662.D
 Acq On : 23 Nov 2021 10:05
 Operator : SY/MD
 Sample : BFB239
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB239

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 26 01:51:50 2021

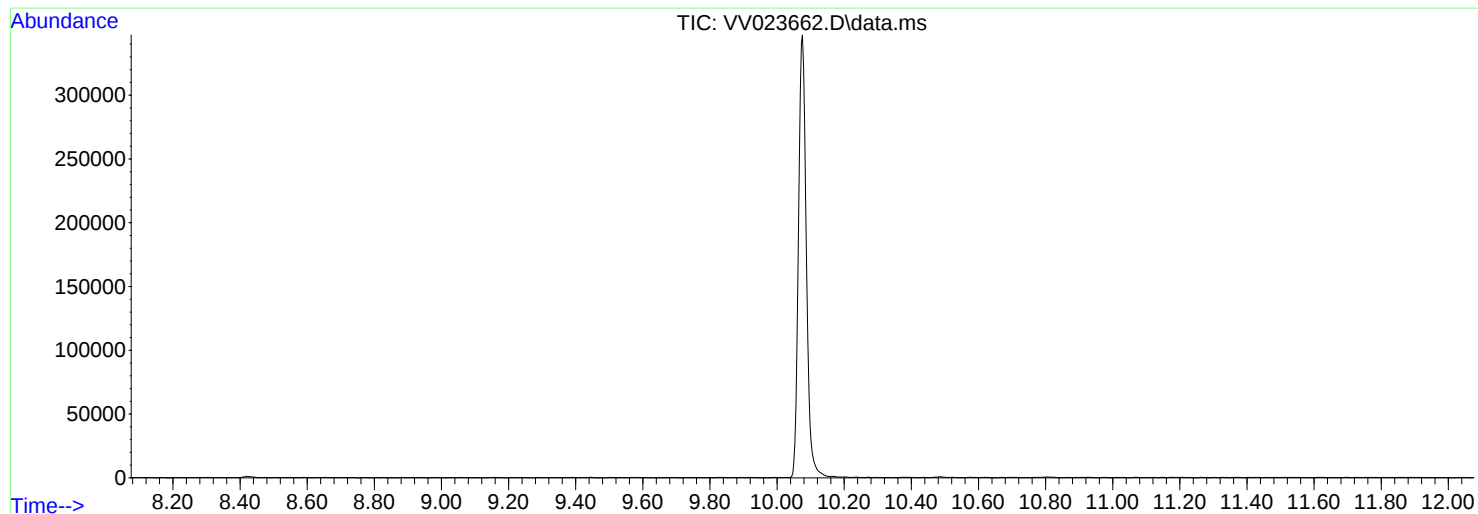

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	10901	PASS
75	95	30	80	48.3	31512	PASS
95	95	100	100	100.0	65253	PASS
96	95	5	9	6.5	4215	PASS
173	174	0.00	2	1.4	844	PASS
174	95	50	120	92.5	60387	PASS
175	174	5	9	7.9	4769	PASS
176	174	95	105	99.6	60117	PASS
177	176	5	10	6.3	3811	PASS

m/z	Abundance
36.00	543.0
37.00	2838.0
38.10	2784.0
39.10	1306.0
39.90	214.0
44.00	471.0
45.10	429.0
47.00	772.0
48.00	338.0
49.00	2503.0
50.10	11224.0
51.10	3563.0
52.00	199.0
53.00	130.0
55.00	199.0
56.10	913.0
57.00	1856.0
60.00	640.0
61.10	3202.0
62.00	3421.0
63.10	3229.0
64.00	489.0
65.00	570.0
66.10	110.0
66.90	167.0
68.00	6318.0
69.00	6879.0
70.00	554.0
72.00	406.0
73.00	3205.0
74.00	11655.0
75.00	32320.0
76.00	2914.0
76.90	432.0
77.90	205.0
78.90	2912.0
80.00	879.0
80.90	2644.0
81.90	673.0
87.00	2671.0
87.90	2841.0
90.90	290.0
92.00	2034.0
93.00	2936.0
94.10	8342.0
95.00	67128.0
96.00	4392.0
96.90	111.0
104.00	397.0
104.90	115.0
105.90	308.0
106.80	105.0
116.00	321.0
116.90	433.0
117.90	323.0
118.90	514.0
127.90	320.0
128.90	114.0
129.90	289.0
134.90	114.0
136.80	151.0
140.90	851.0
141.80	108.0
143.00	1278.0
143.80	101.0
144.90	496.0
145.90	133.0
148.00	215.0
148.90	110.0
155.00	224.0
156.90	217.0
171.30	191.0
172.00	745.0
173.10	886.0
174.00	62296.0
175.00	4965.0
176.00	62048.0
177.00	3841.0
178.10	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

Scan 2796 (10.030 min): VV023662.D\data.ms
BFB239

m/z	Abundance
40.00	133.0
43.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.00	538.0
37.10	2873.0
38.00	2736.0
39.10	1283.0
39.90	242.0
44.00	464.0
45.10	403.0
45.90	124.0
47.00	692.0
48.00	364.0
49.00	2592.0
50.10	10742.0
51.00	3471.0
52.00	161.0
53.00	140.0
55.10	271.0
56.00	977.0
57.00	1862.0
58.20	119.0
60.00	684.0
61.10	3154.0
62.00	3544.0
63.00	3234.0
64.00	449.0
65.00	616.0
66.10	110.0
67.00	194.0
68.00	6357.0
69.00	6905.0
70.00	540.0
72.00	442.0
73.00	3169.0
74.00	11353.0
75.00	31856.0
76.00	2831.0
77.00	446.0
77.90	286.0
78.90	2876.0
79.90	845.0
81.00	2691.0
81.90	715.0
86.20	124.0
87.00	2695.0
88.00	2892.0
90.90	304.0
92.00	2018.0
93.00	2859.0
94.00	8329.0
95.00	66096.0
96.00	4452.0
96.90	120.0
104.00	418.0
105.80	282.0
106.80	116.0
109.90	103.0
115.90	324.0
116.90	489.0
117.90	304.0
118.90	490.0
127.90	263.0
128.90	128.0
129.90	352.0
134.90	121.0
136.80	144.0
140.90	798.0
141.80	109.0
143.00	1293.0
143.80	107.0
144.90	483.0
145.90	143.0
148.00	215.0
148.90	116.0
155.00	180.0
156.90	175.0
160.90	106.0
171.20	168.0
172.00	635.0
173.10	814.0
174.00	60168.0
175.00	4911.0
176.00	59760.0
177.00	3858.0
178.00	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.10	510.0
37.00	2564.0
38.10	2636.0
39.10	1189.0
39.90	163.0
44.00	419.0
45.00	438.0
47.00	720.0
48.00	321.0
49.00	2303.0
50.10	10736.0
51.10	3371.0
51.90	211.0
52.90	104.0
55.10	143.0
56.10	784.0
57.00	1742.0
60.00	564.0
61.00	2921.0
62.00	3023.0
63.10	2831.0
64.00	469.0
65.10	537.0
66.90	162.0
68.00	5932.0
69.00	6317.0
70.10	498.0
72.00	326.0
73.00	3009.0
74.00	11007.0
75.00	30360.0
76.00	2691.0
76.90	387.0
78.10	198.0
79.00	2738.0
79.90	800.0
80.90	2433.0
82.00	589.0
82.90	103.0
87.00	2415.0
87.90	2501.0
90.90	280.0
92.10	1861.0
93.00	2860.0
94.00	7695.0
95.00	62536.0
96.10	3801.0
104.00	349.0
104.80	130.0
105.90	330.0
116.00	296.0
116.90	416.0
117.90	292.0
119.00	487.0
127.90	365.0
128.90	108.0
129.80	241.0
134.90	105.0
136.80	155.0
140.90	846.0
141.90	106.0
143.00	1090.0
143.80	103.0
144.80	450.0
145.90	117.0
148.00	193.0
155.00	219.0
156.90	215.0
172.00	785.0
173.10	833.0
174.00	58696.0
175.00	4432.0
176.00	58544.0
177.00	3734.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239