


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112421\  
Data File : VV023698.D  
Acq On : 24 Nov 2021 14:17  
Operator : SY/MD  
Sample : M4821-01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
Client Sampled :  
H4635

Quant Time: Nov 26 01:53:20 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Nov 26 01:51:50 2021  
Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021  
Supervised By : Mahesh Dadoda 11/26/2021

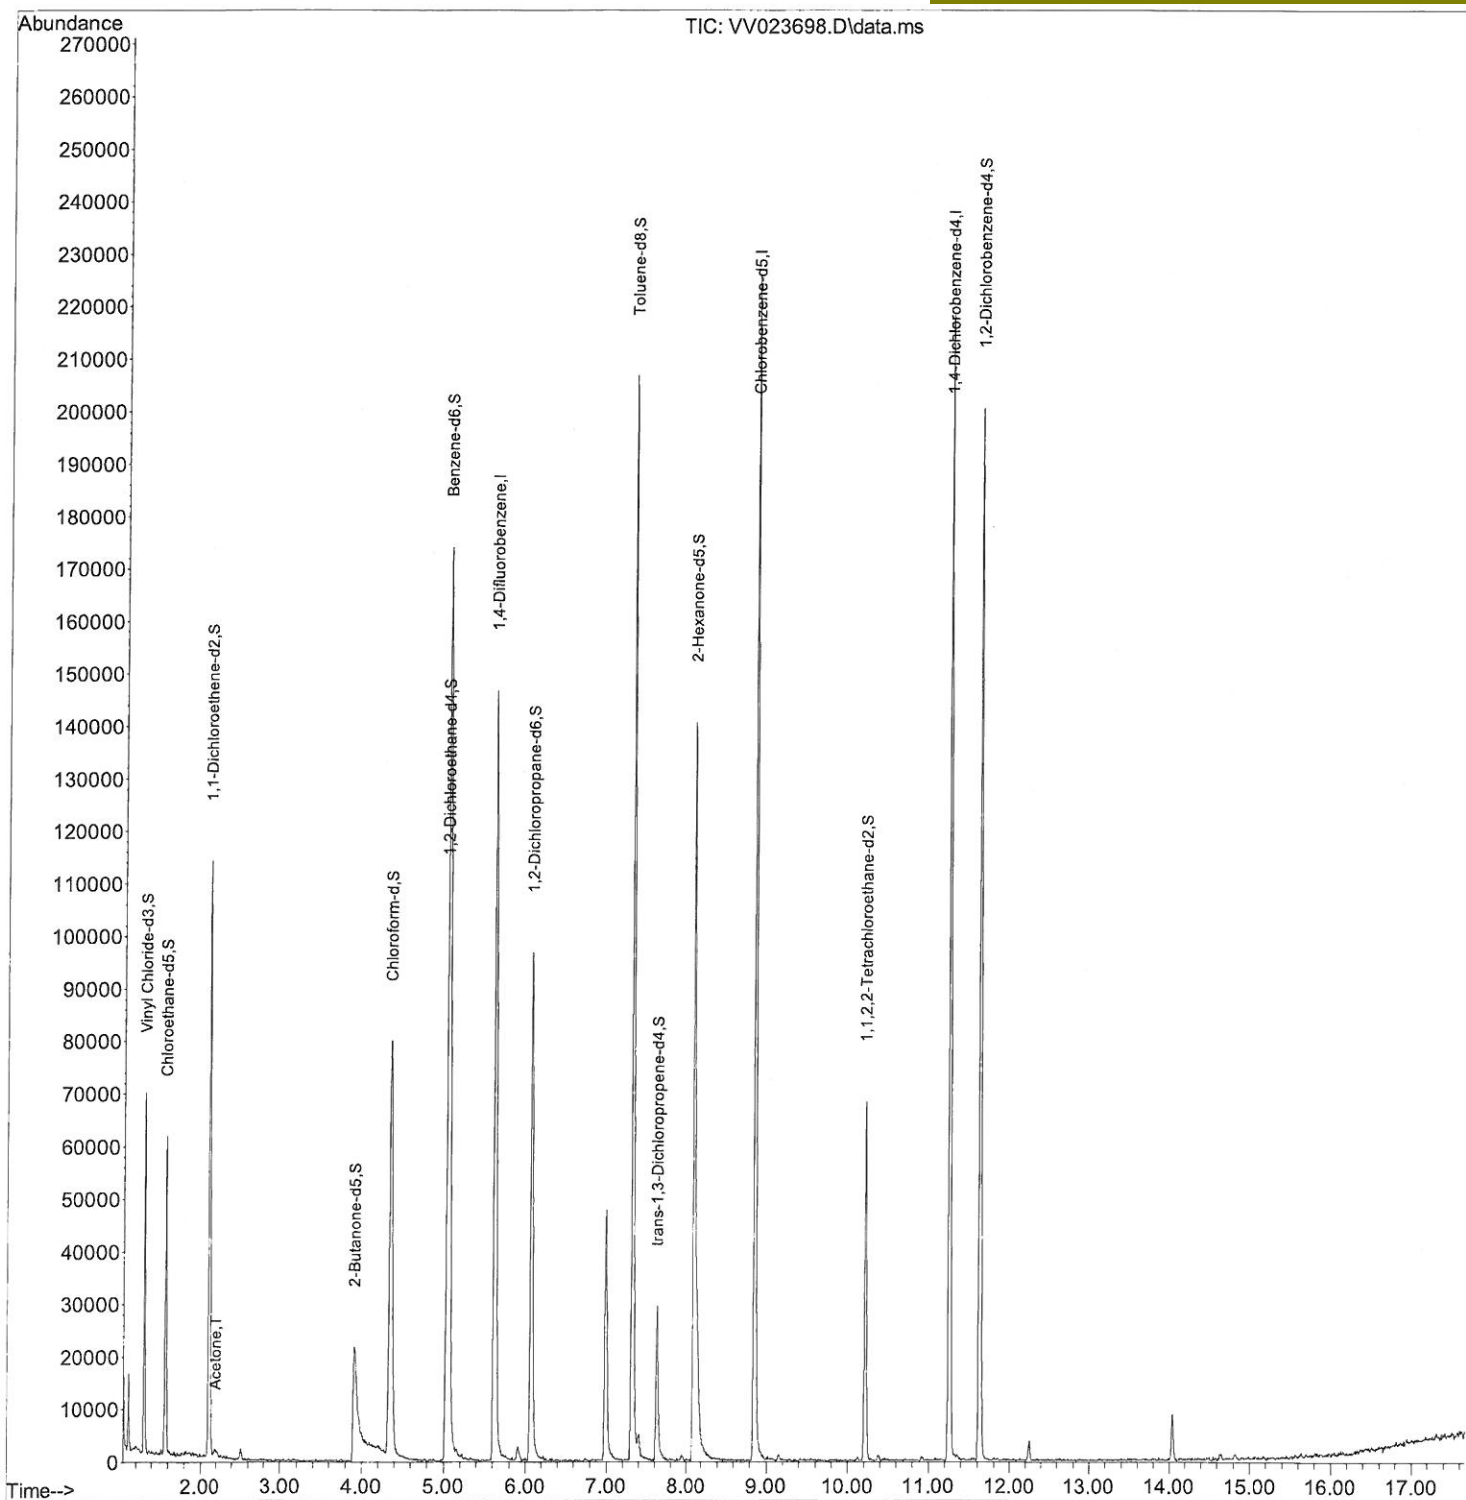

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112421\  
 Data File : VV023698.D  
 Acq On : 24 Nov 2021 14:17  
 Operator : SY/MD  
 Sample : M4821-01  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sample Id :  
 H4635

Quant Time: Nov 26 01:53:20 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 26 01:51:50 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021  
 Supervised By : Mahesh Dadoda 11/26/2021

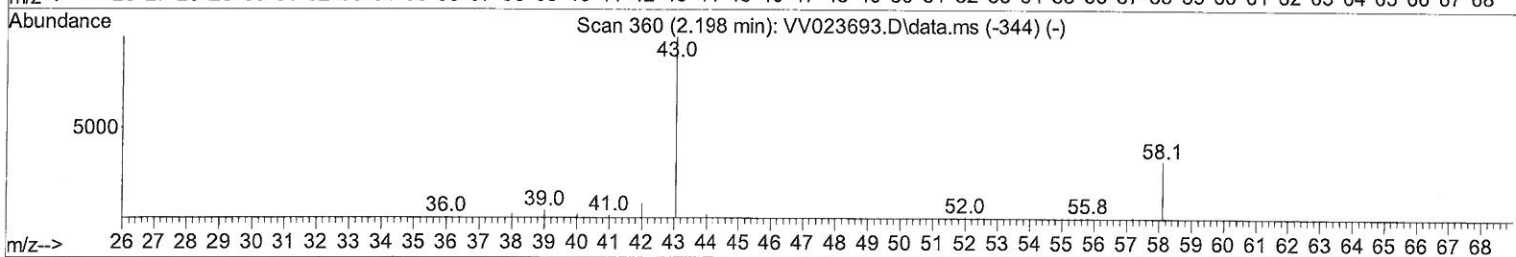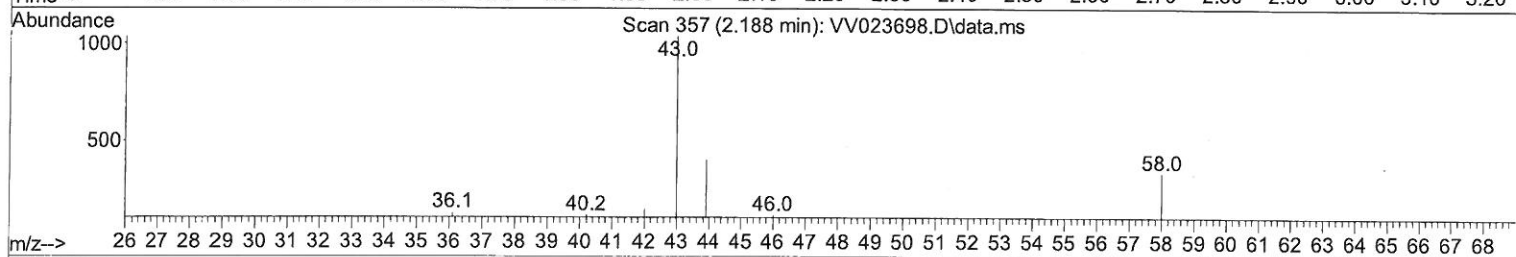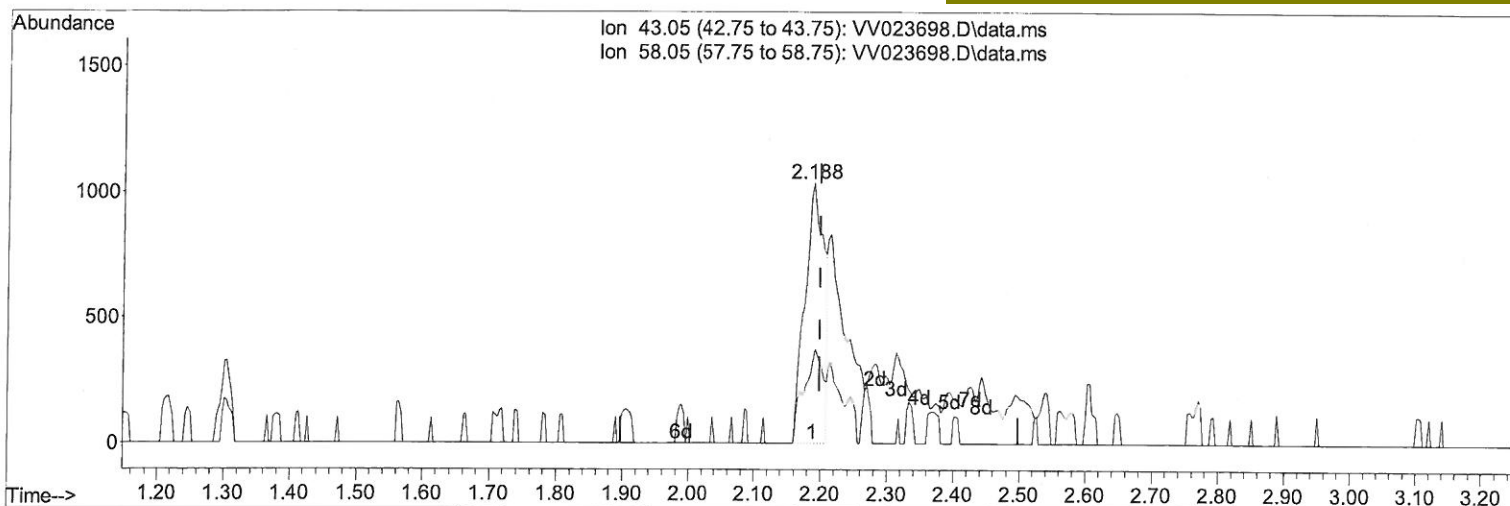

TIC: VV023698.D\data.ms

(13) Acetone (T)

2.188min (-0.010) 1.72 ug/L

response 2002

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	36.96
0.00	0.00	0.00
0.00	0.00	0.00

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112421\  
 Data File : VV023698.D  
 Acq On : 24 Nov 2021 14:17  
 Operator : SY/MD  
 Sample : M4821-01  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sample Id :  
 H4635

Quant Time: Nov 26 01:53:20 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 26 01:51:50 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021  
 Supervised By : Mahesh Dadoda 11/26/2021

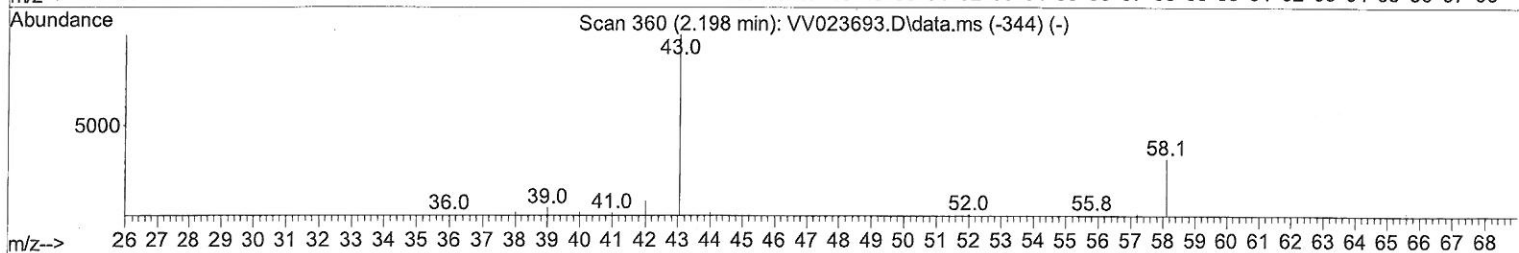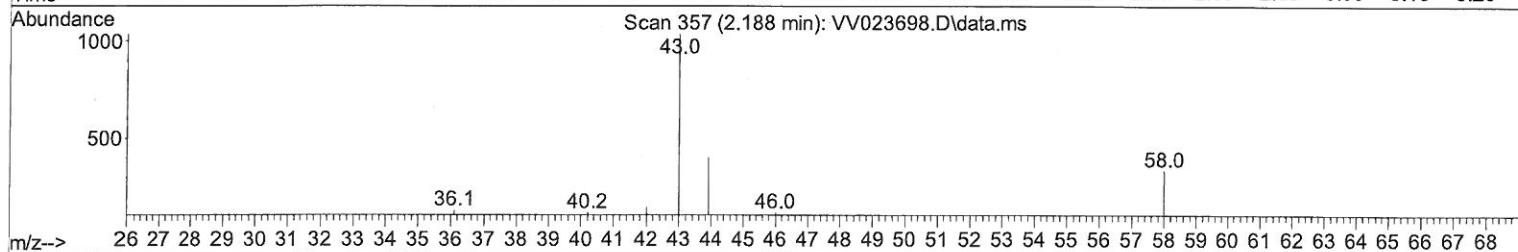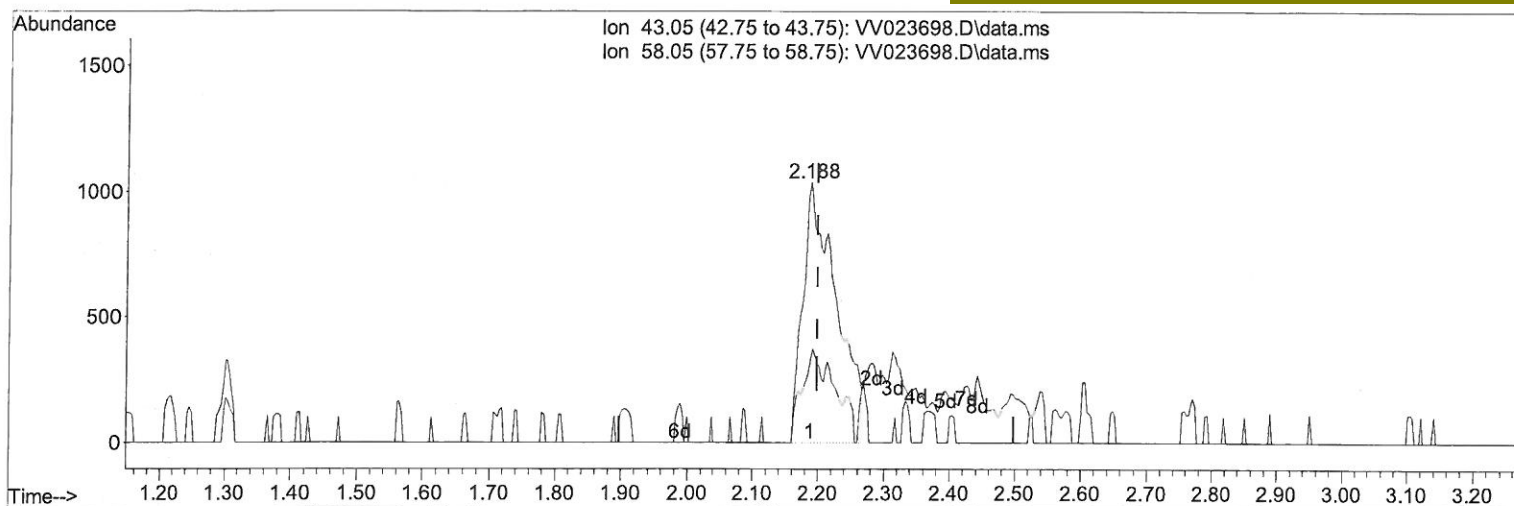

TIC: VV023698.D\data.ms

(13) Acetone (T)

2.188min (-0.010) 3.14 ug/L m

response 3659

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	20.22
0.00	0.00	0.00
0.00	0.00	0.00

*MD*  
*12/01/21*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112421\  
 Data File : VV023698.D  
 Acq On : 24 Nov 2021 14:17  
 Operator : SY/MD  
 Sample : M4821-01  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sampled :  
 H4635

Quant Time: Nov 26 01:53:20 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 26 01:51:50 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021  
 Supervised By : Mahesh Dadoda 11/26/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	131264	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	126185	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59047	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	42076	3.905	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.000%	
7) Chloroethane-d5	1.565	69	35490	4.190	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.800%	
11) 1,1-Dichloroethene-d2	2.105	63	58559	3.084	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.600%	
20) 2-Butanone-d5	3.905	46	52163	40.268	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	80.540%	
24) Chloroform-d	4.346	84	81414	4.339	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.800%	
26) 1,2-Dichloroethane-d4	5.031	65	39818	4.542	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
32) Benzene-d6	5.050	84	159312	4.635	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	6.069	67	46228	4.797	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.000%	
41) Toluene-d8	7.317	98	137287	4.275	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.400%	
43) trans-1,3-Dichloroprop...	7.625	79	18361	4.727	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.092	63	61252	47.461	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.920%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31642	4.563	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	54251	5.197	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.000%	
Target Compounds						
13) Acetone	2.188	43	3659m	3.139	ug/L	Qvalue

7 MD  
 12/01/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed