

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112421\
 Data File : VW023698.D
 Acq On : 24 Nov 2021 14:17
 Operator : SY/MD
 Sample : M4821-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4635

Manual Integrations
 APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Mahesh Dadoda 11/26/2021

Quant Time: Nov 26 01:53:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 01:51:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	131264	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	126185	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59047	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	42076	3.905	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.000%	
7) Chloroethane-d5	1.565	69	35490	4.190	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.800%	
11) 1,1-Dichloroethene-d2	2.105	63	58559	3.084	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.600%	
20) 2-Butanone-d5	3.905	46	52163	40.268	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	80.540%	
24) Chloroform-d	4.346	84	81414	4.339	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.800%	
26) 1,2-Dichloroethane-d4	5.031	65	39818	4.542	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
32) Benzene-d6	5.050	84	159312	4.635	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	6.069	67	46228	4.797	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.000%	
41) Toluene-d8	7.317	98	137287	4.275	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.400%	
43) trans-1,3-Dichloroprop...	7.625	79	18361	4.727	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.092	63	61252	47.461	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.920%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31642	4.563	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	54251	5.197	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.000%	
Target Compounds					Qvalue	
13) Acetone	2.188	43	3659m	3.139	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023698.D
Acq On : 24 Nov 2021 14:17
Operator : SY/MD
Sample : M4821-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
H4635

Manual Integrations
APPROVED

Reviewed By : John Carlone 11/26/2021
Supervised By : Mahesh Dadoda 11/26/2021


Quant Time: Nov 26 01:53:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 26 01:51:50 2021
Response via : Initial Calibration

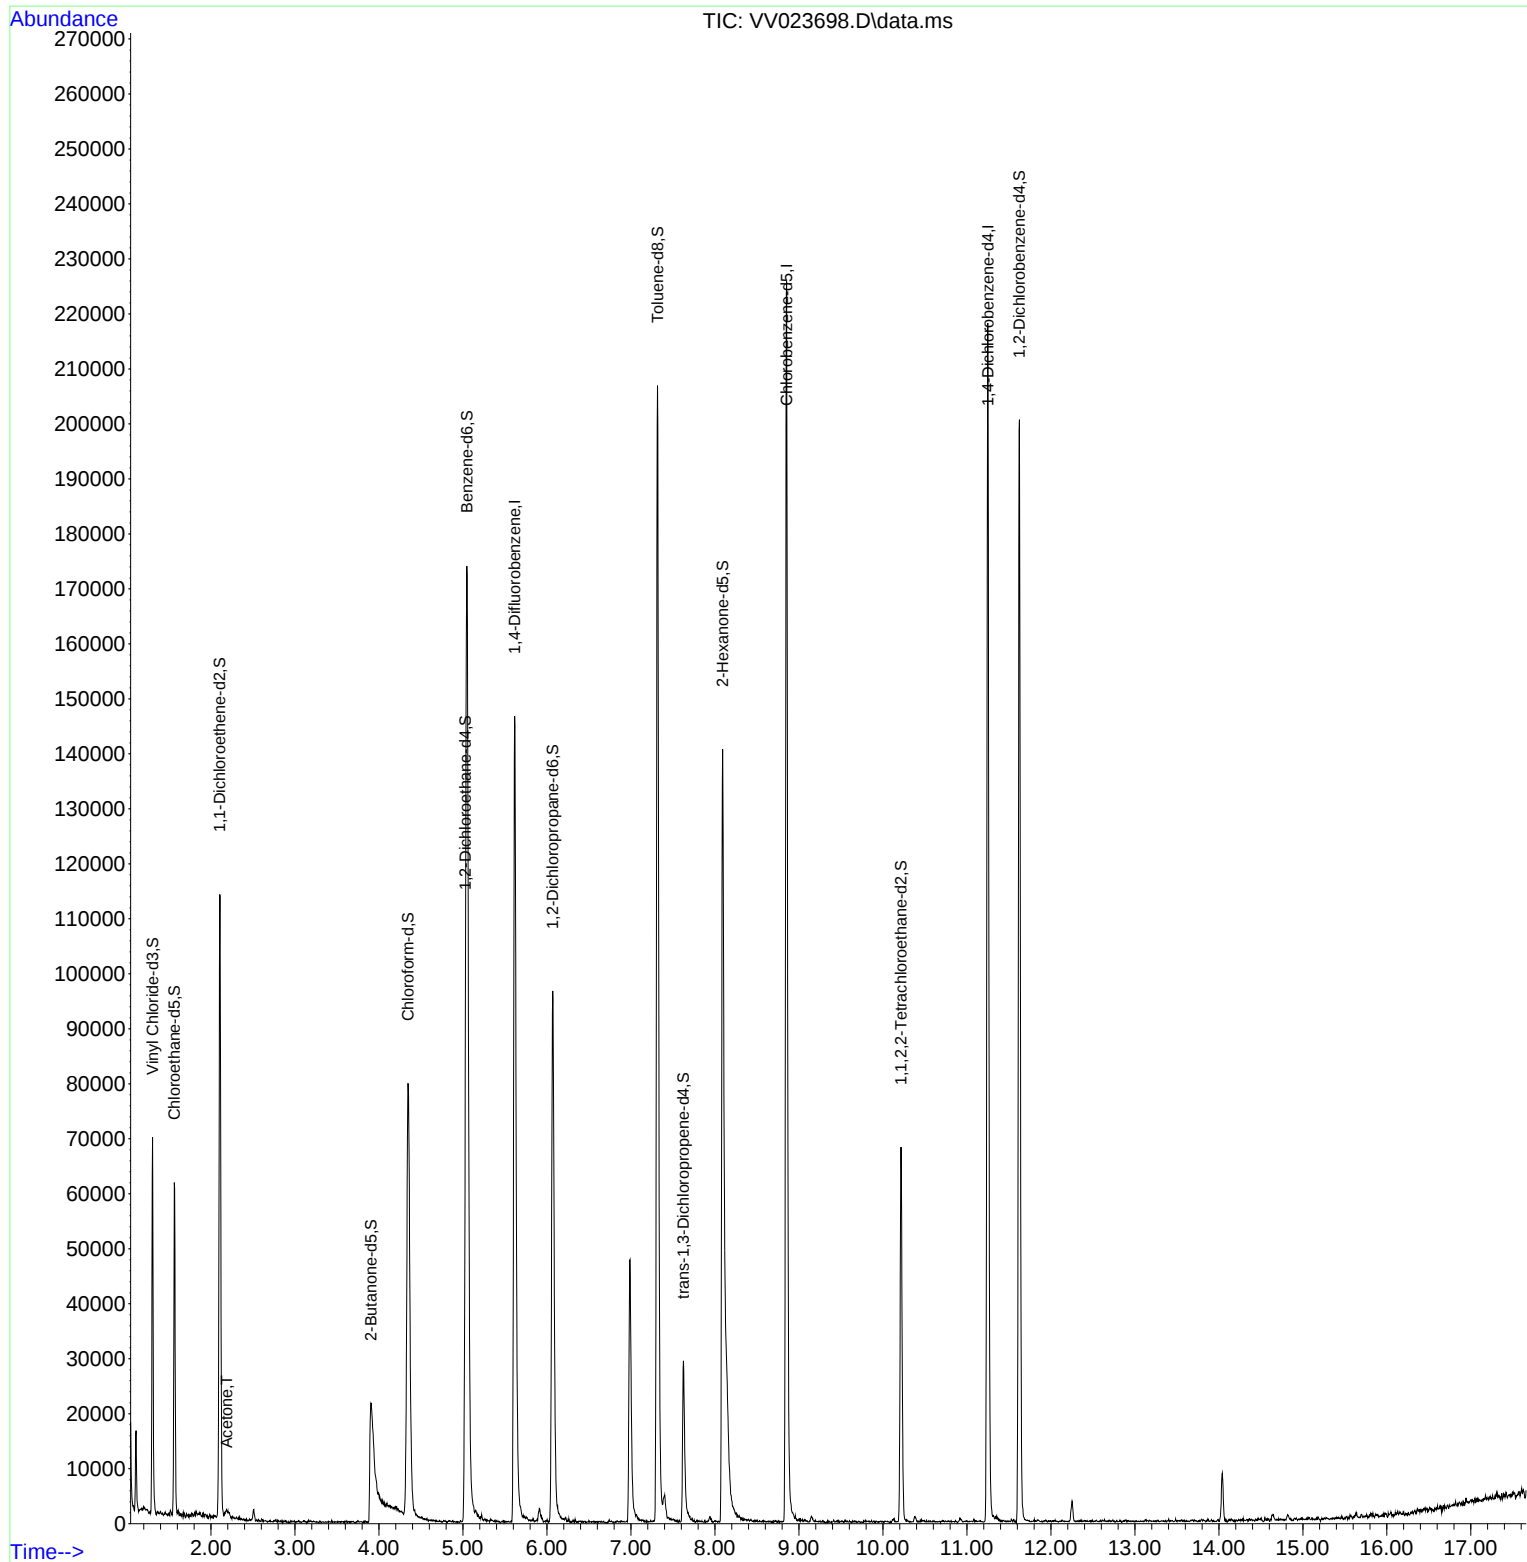

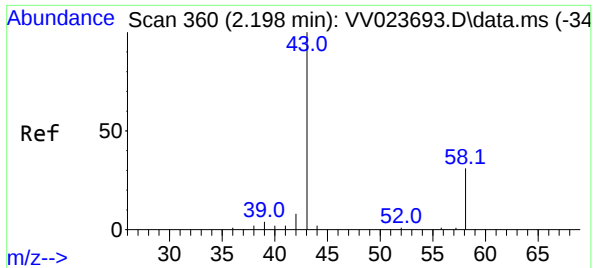

#13
 Acetone
 Concen: 3.139 ug/L m
 RT: 2.188 min Scan# 3
 Delta R.T. -0.010 min
 Lab File: VV023698.D
 Acq: 24 Nov 2021 14:17

Instrument :
 MSVOA_V
 ClientSampleId :
 H4635

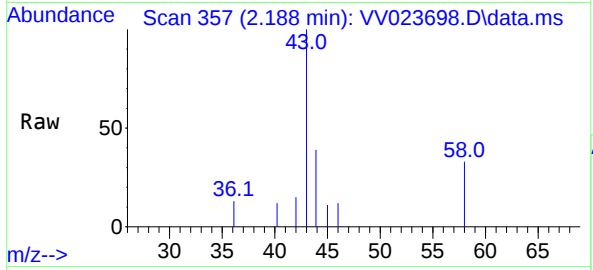

Tgt Ion: 43 Resp: 365

Ion	Ratio	Lower	Upper
43	100		
58	20.2	0.0	41.4

Manual Integrations
 APPROVED

Reviewed By :John Carlone 11/26/2021
 Supervised By :Mahesh Dadoda 11/26/2021

