

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023695.D
Acq On : 24 Nov 2021 13:06
Operator : SY/MD
Sample : M4723-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G43DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Title : TRACE VOA SFAM1.0

Signal : TIC: VV023695.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	13	20	45	rBV	36380774	51915026	100.00%	98.042%
2	1.214	45	54	73	rVB	957988	1037055	2.00%	1.958%




Sum of corrected areas: 52952081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023695.D
Acq On : 24 Nov 2021 13:06
Operator : SY/MD
Sample : M4723-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

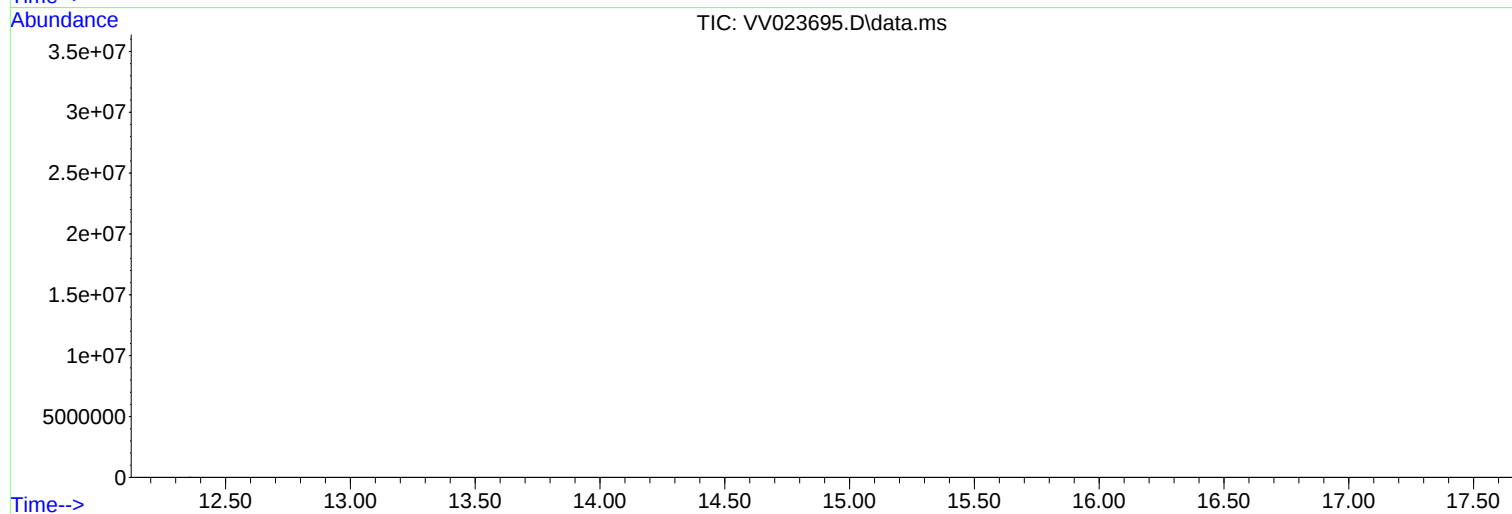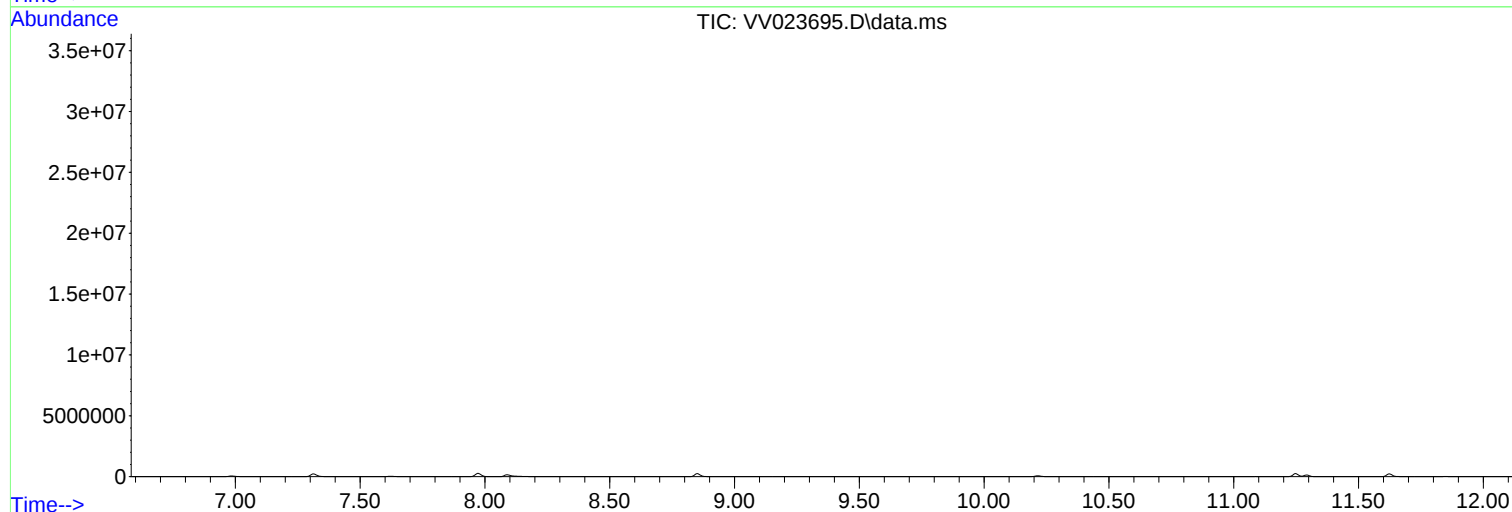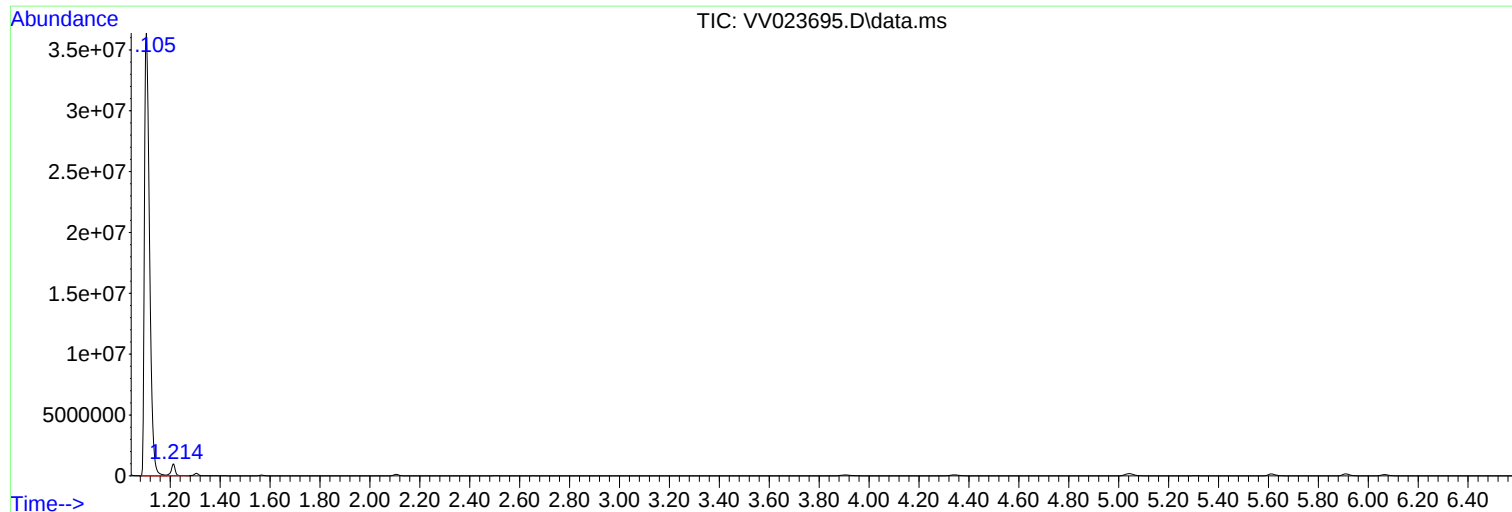

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023695.D
Acq On : 24 Nov 2021 13:06
Operator : SY/MD
Sample : M4723-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G43DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.105	250.30 ug/L	51915000	1,4-Difluorobenzene	5.613

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane	44	C3H8	000074-98-6	83
2			Propane	44	C3H8	000074-98-6	56
3			Propane	44	C3H8	000074-98-6	9
4			Propene	42	C3H6	000115-07-1	9
5			Ethylene oxide	44	C2H4O	000075-21-8	5

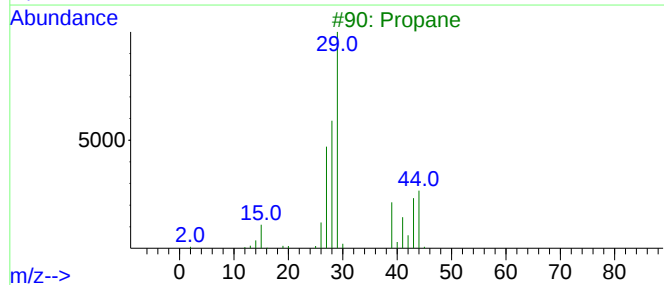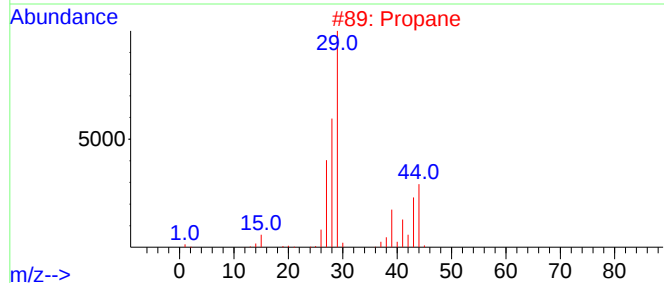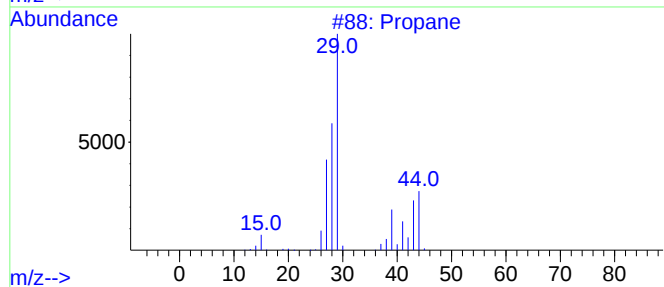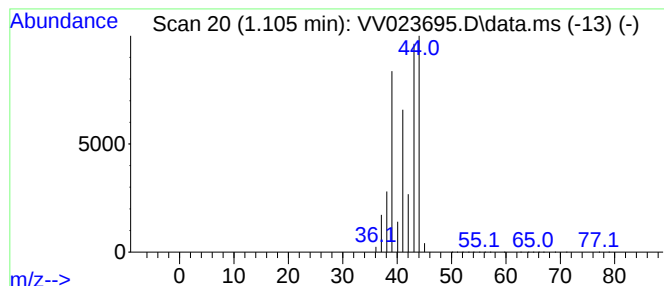

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023695.D
Acq On : 24 Nov 2021 13:06
Operator : SY/MD
Sample : M4723-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G43DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.214	5.00 ug/L	1037060	1,4-Difluorobenzene	5.613

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Isobutane	58	C4H10	000075-28-5	64
2		Isobutane	58	C4H10	000075-28-5	64
3		Isobutane	58	C4H10	000075-28-5	64
4		Isobutane	58	C4H10	000075-28-5	53
5		Isobutane	58	C4H10	000075-28-5	50

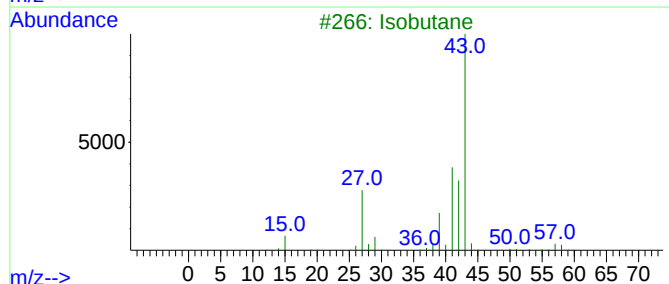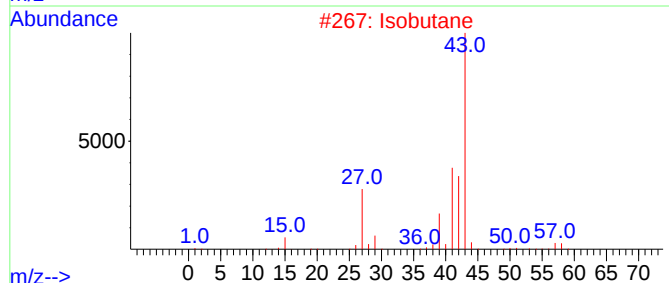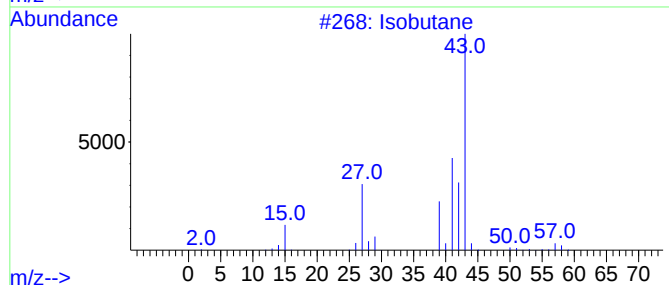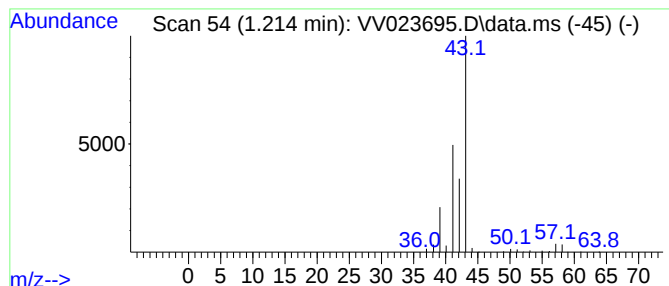

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023695.D
Acq On : 24 Nov 2021 13:06
Operator : SY/MD
Sample : M4723-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.105	250.3	ug/L	51915000	1	5.613	1037060	5.0
(DEL) Alkane: S...	1.214	5.0	ug/L	1037060	1	5.613	1037060	5.0