

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
 Data File : VV023698.D
 Acq On : 24 Nov 2021 14:17
 Operator : SY/MD
 Sample : M4821-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4635

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	15	21	30	rVB	14777	14483	3.28%	0.406%
2	1.304	75	82	97	rVB	68681	70456	15.96%	1.973%
3	1.565	155	163	173	rBV	60465	67657	15.33%	1.894%
4	2.105	320	331	345	rBV	113207	163106	36.95%	4.567%
5	3.905	881	891	917	rBV2	21677	81226	18.40%	2.274%
6	4.346	1012	1028	1051	rBV3	78300	200209	45.36%	5.606%
7	5.047	1228	1246	1275	rBV2	173798	441413	100.00%	12.359%
8	5.616	1412	1423	1454	rBV	146544	299874	67.94%	8.396%
9	6.069	1550	1564	1581	rBV	96572	201469	45.64%	5.641%
10	6.989	1840	1850	1871	rBV2	47667	91569	20.74%	2.564%
11	7.317	1940	1952	1971	rBV	206497	363334	82.31%	10.173%
12	7.404	1971	1979	1988	rVB6	4302	8775	1.99%	0.246%
13	7.625	2036	2048	2065	rBV2	29333	52760	11.95%	1.477%
14	8.092	2181	2193	2241	rBV	140575	352671	79.90%	9.875%
15	8.854	2417	2430	2460	rBV	225516	371256	84.11%	10.395%
16	10.217	2843	2854	2873	rBV	68106	108740	24.63%	3.045%
17	11.249	3160	3175	3193	rBV	218055	344485	78.04%	9.646%
18	11.625	3281	3292	3311	rBV	200504	318448	72.14%	8.916%
19	12.252	3479	3487	3498	rVB3	3707	5540	1.26%	0.155%
20	14.040	4033	4043	4056	rVB	8763	13984	3.17%	0.392%




Sum of corrected areas: 3571455

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023698.D
Acq On : 24 Nov 2021 14:17
Operator : SY/MD
Sample : M4821-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

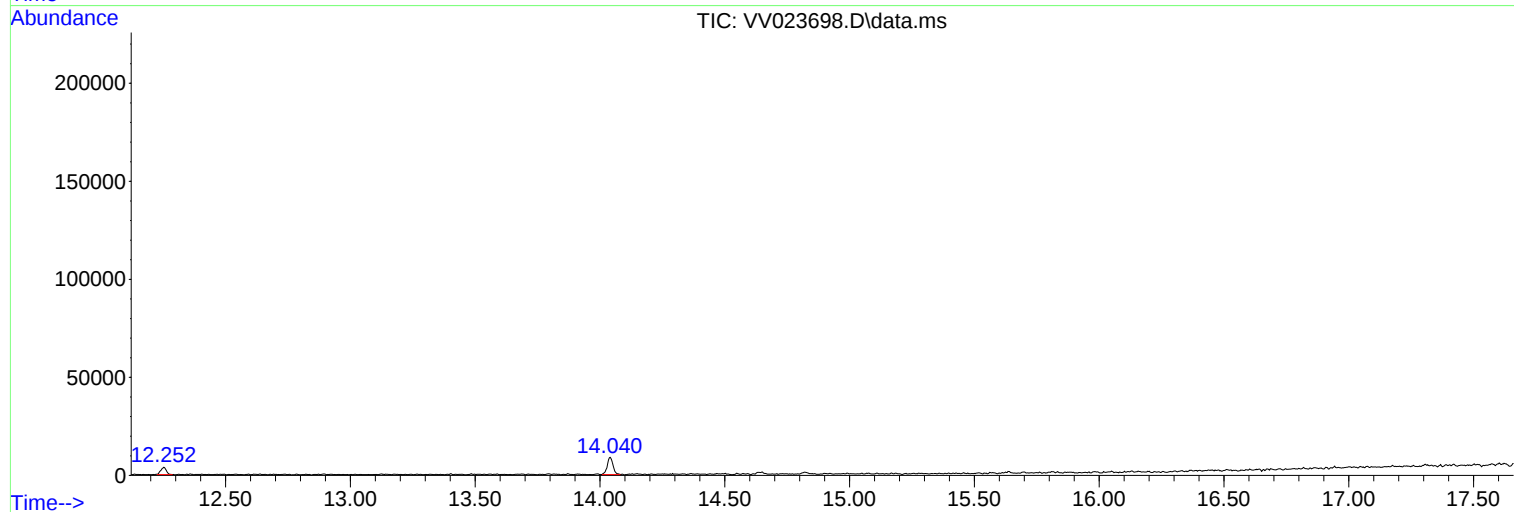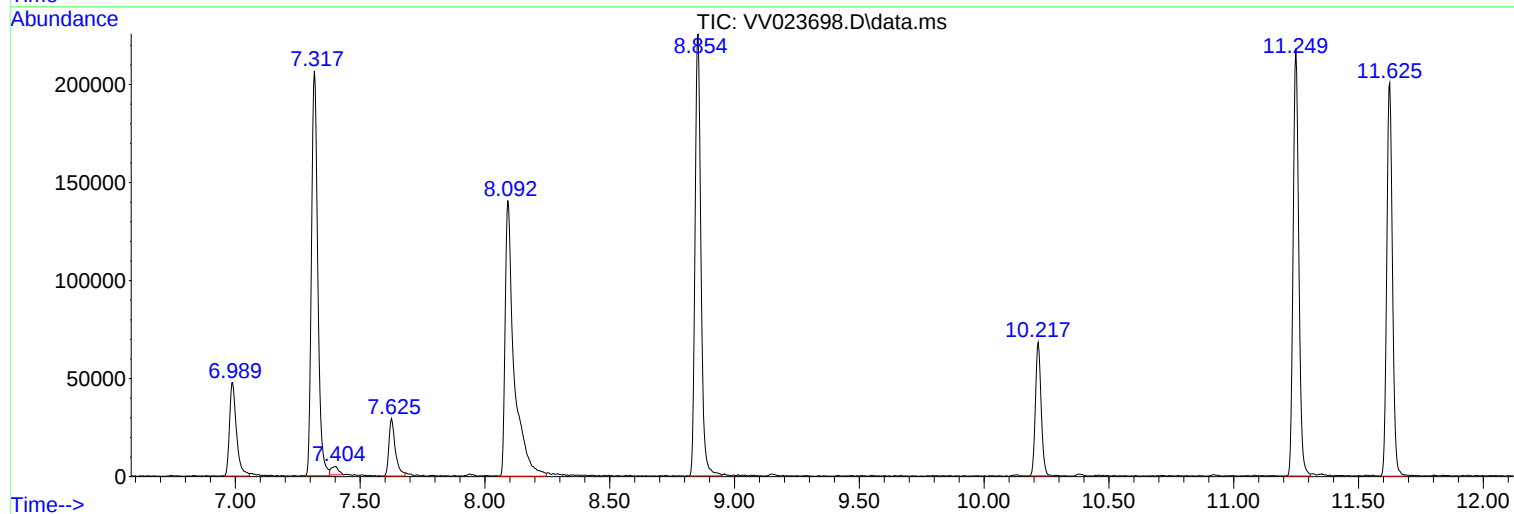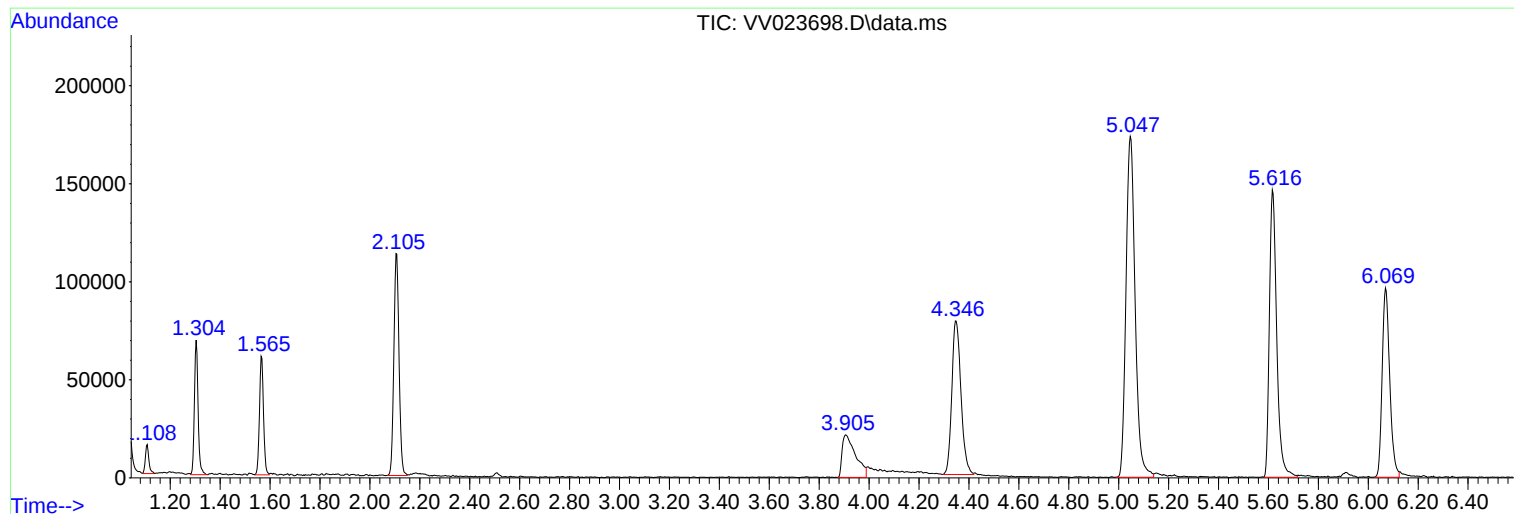

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023698.D
Acq On : 24 Nov 2021 14:17
Operator : SY/MD
Sample : M4821-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023698.D
Acq On : 24 Nov 2021 14:17
Operator : SY/MD
Sample : M4821-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc