

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
 Data File : VV023704.D
 Acq On : 24 Nov 2021 16:40
 Operator : SY/MD
 Sample : M4821-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4655

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	44	rVB	123463	123777	12.46%	2.240%
2	1.307	76	83	94	rBV	65011	68676	6.91%	1.243%
3	1.568	157	164	178	rBV	60641	70530	7.10%	1.277%
4	2.108	322	332	347	rVB	117597	168048	16.92%	3.042%
5	2.767	519	537	561	rBV	463864	993417	100.00%	17.982%
6	3.905	879	891	914	rBV3	39336	139683	14.06%	2.528%
7	4.349	1013	1029	1057	rBV	74791	201846	20.32%	3.654%
8	5.050	1229	1247	1274	rBV3	172013	441340	44.43%	7.989%
9	5.616	1412	1423	1448	rBV	152414	314623	31.67%	5.695%
10	5.918	1505	1517	1537	rBV3	25618	54832	5.52%	0.992%
11	6.069	1549	1564	1596	rBV2	99110	210126	21.15%	3.803%
12	6.989	1840	1850	1866	rBV	47140	90248	9.08%	1.634%
13	7.317	1941	1952	1973	rBV	201524	355566	35.79%	6.436%
14	7.625	2039	2048	2068	rBV2	28177	53281	5.36%	0.964%
15	7.973	2139	2156	2177	rBV	402748	671898	67.64%	12.162%
16	8.092	2183	2193	2219	rBV	185353	375837	37.83%	6.803%
17	8.850	2418	2429	2450	rBV	235298	387921	39.05%	7.022%
18	10.217	2843	2854	2873	rBV	73449	118729	11.95%	2.149%
19	11.249	3164	3175	3198	rBV	231961	361269	36.37%	6.539%
20	11.625	3280	3292	3310	rBV	204722	322999	32.51%	5.847%




Sum of corrected areas: 5524646

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023704.D
Acq On : 24 Nov 2021 16:40
Operator : SY/MD
Sample : M4821-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

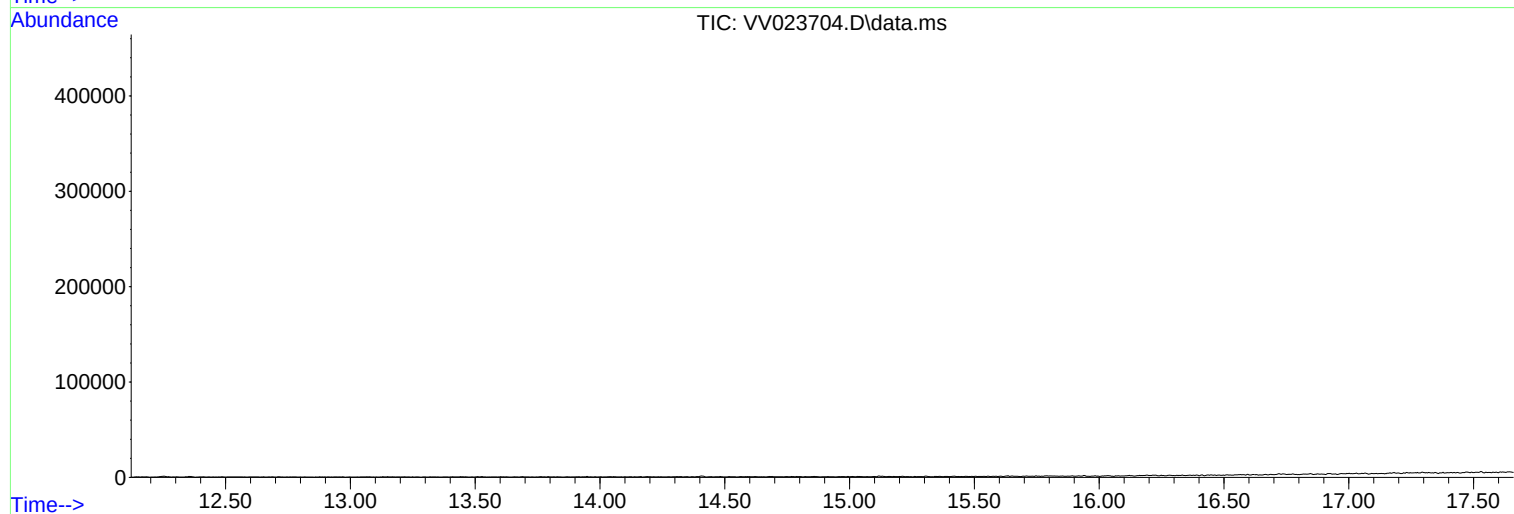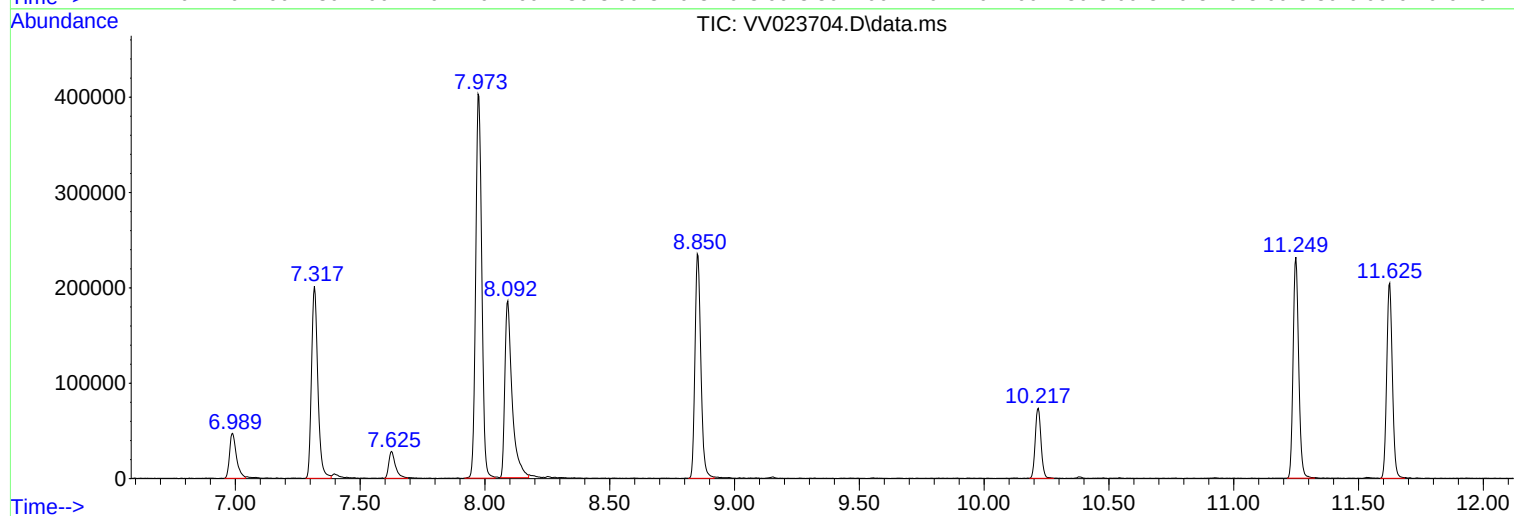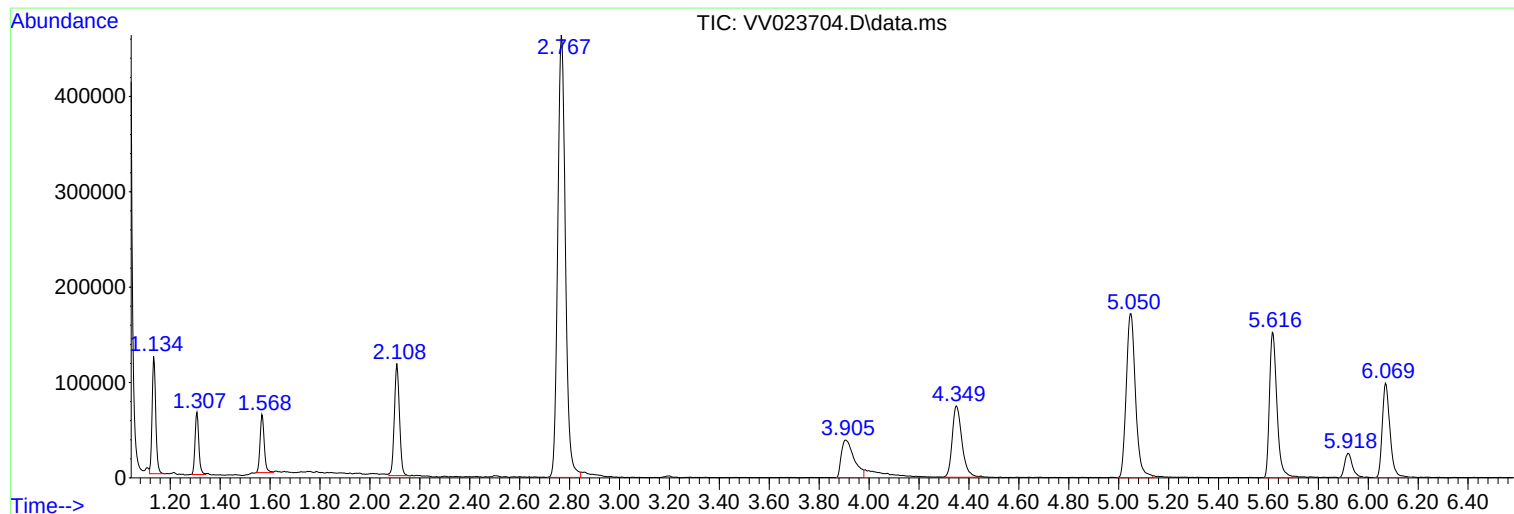

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023704.D
Acq On : 24 Nov 2021 16:40
Operator : SY/MD
Sample : M4821-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023704.D
Acq On : 24 Nov 2021 16:40
Operator : SY/MD
Sample : M4821-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
