

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
 Data File : VV023707.D
 Acq On : 24 Nov 2021 17:51
 Operator : SY/MD
 Sample : M4821-09MS
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4657MS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	73	84	103	rVB2	147487	174462	1.36%	0.580%
2	1.754	213	222	240	rVB	175066	224732	1.75%	0.747%
3	2.117	323	335	348	rBV4	357013	607537	4.72%	2.018%
4	2.294	380	390	405	rVB	132533	197191	1.53%	0.655%
5	2.506	446	456	478	rVB	117024	199936	1.55%	0.664%
6	2.767	519	537	561	rBV	6091808	12866748	100.00%	42.743%
7	3.191	654	669	694	rVB	92584	195262	1.52%	0.649%
8	3.912	878	893	908	rBV2	131400	355556	2.76%	1.181%
9	4.249	986	998	1015	rVV2	59150	141904	1.10%	0.471%
10	4.368	1016	1035	1060	rVB4	119682	421768	3.28%	1.401%
11	4.612	1092	1111	1121	rBV	109987	279938	2.18%	0.930%
12	4.680	1121	1132	1152	rVB2	145653	360149	2.80%	1.196%
13	4.831	1160	1179	1202	rVB2	109543	260702	2.03%	0.866%
14	5.050	1229	1247	1255	rBV2	172066	419356	3.26%	1.393%
15	5.101	1256	1263	1295	rVB3	200246	541611	4.21%	1.799%
16	5.619	1411	1424	1443	rBV	153922	311566	2.42%	1.035%
17	5.915	1503	1516	1545	rBV	163496	327237	2.54%	1.087%
18	6.069	1552	1564	1573	rBV2	95154	190830	1.48%	0.634%
19	6.130	1573	1583	1591	rVV	200308	423191	3.29%	1.406%
20	6.172	1592	1596	1614	rVB2	122686	214914	1.67%	0.714%
21	6.509	1688	1701	1726	rBV	98271	190547	1.48%	0.633%
22	7.027	1855	1862	1884	rVB	106695	206759	1.61%	0.687%
23	7.226	1912	1924	1942	rBV	320008	628016	4.88%	2.086%
24	7.317	1942	1952	1964	rVV	223113	415472	3.23%	1.380%
25	7.387	1964	1974	1997	rVB	314816	546833	4.25%	1.817%
26	7.651	2038	2056	2084	rBV2	103008	234658	1.82%	0.780%
27	7.841	2103	2115	2137	rBV	107410	188477	1.46%	0.626%
28	7.976	2141	2157	2183	rVB	216903	366008	2.84%	1.216%
29	8.091	2183	2193	2201	rBV	177977	320641	2.49%	1.065%
30	8.140	2201	2208	2231	rVV	241021	511928	3.98%	1.701%
31	8.246	2231	2241	2262	rVV	89785	165744	1.29%	0.551%
32	8.853	2419	2430	2434	rBV	250202	388718	3.02%	1.291%
33	8.879	2435	2438	2462	rVB	271577	394296	3.06%	1.310%
34	9.011	2467	2479	2504	rVB	342335	546135	4.24%	1.814%
35	9.140	2506	2519	2541	rBV	332987	547985	4.26%	1.820%
36	9.551	2633	2647	2682	rBV4	448794	1022776	7.95%	3.398%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
 Data File : VV023707.D
 Acq On : 24 Nov 2021 17:51
 Operator : SY/MD
 Sample : M4821-09MS
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4657MS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

37	9.931	2753	2765	2790	rBV	385696	601180	4.67%	1.997%
38	10.538	2942	2954	2974	rBV	386757	582108	4.52%	1.934%
39	10.914	3059	3071	3093	rBV	387829	578380	4.50%	1.921%
40	11.181	3142	3154	3165	rBV	295214	456070	3.54%	1.515%
41	11.249	3165	3175	3178	rBV	303630	412471	3.21%	1.370%
42	11.638	3280	3296	3315	rBV2	329037	760149	5.91%	2.525%
43	12.644	3597	3609	3625	rBV	302797	457495	3.56%	1.520%
44	13.262	3789	3801	3817	rBV	230177	351957	2.74%	1.169%
45	13.503	3866	3876	3896	rVB	120227	188886	1.47%	0.627%
46	13.744	3939	3951	3968	rVB	211635	324609	2.52%	1.078%




Sum of corrected areas: 30102888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023707.D
Acq On : 24 Nov 2021 17:51
Operator : SY/MD
Sample : M4821-09MS
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4657MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

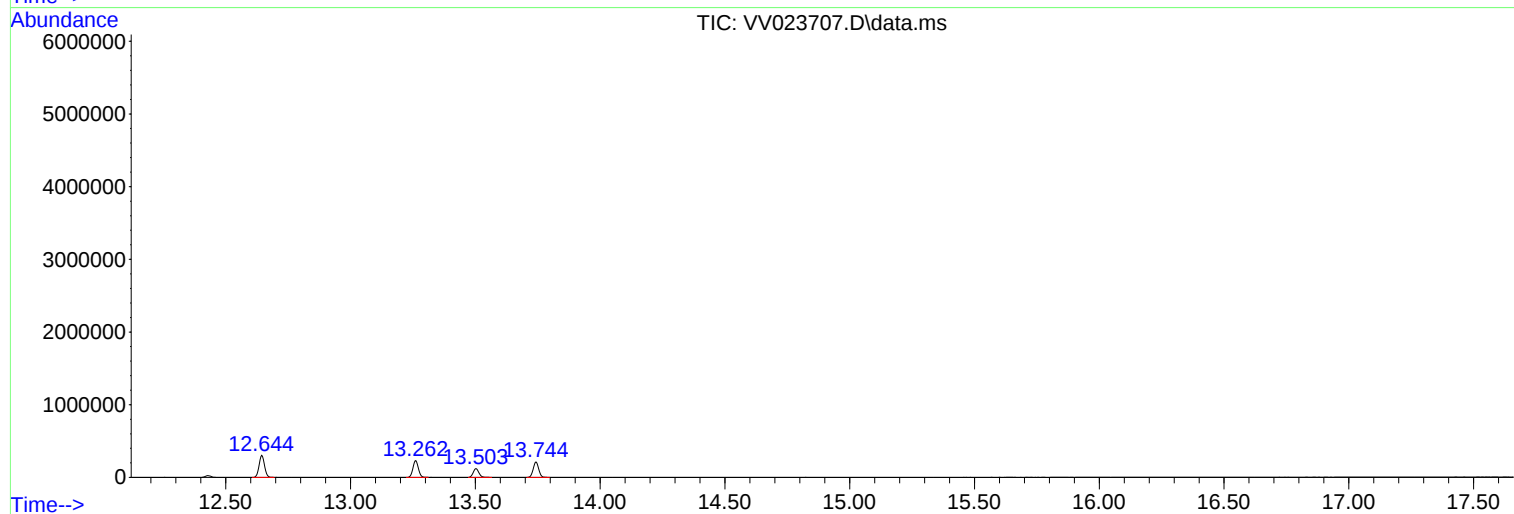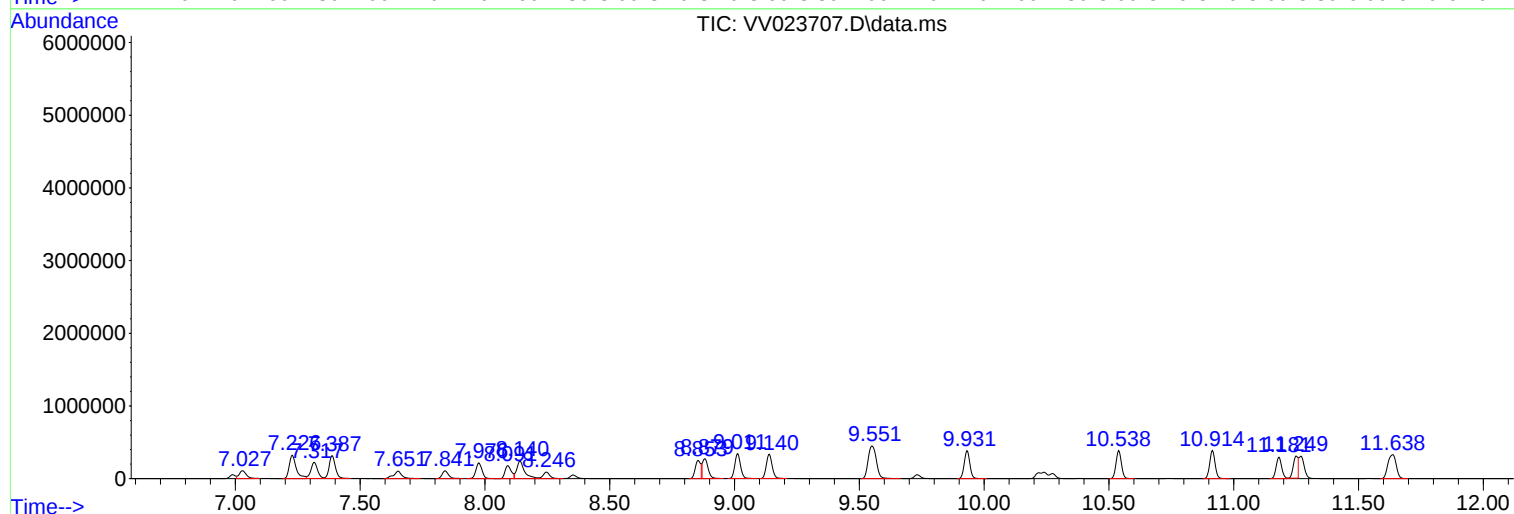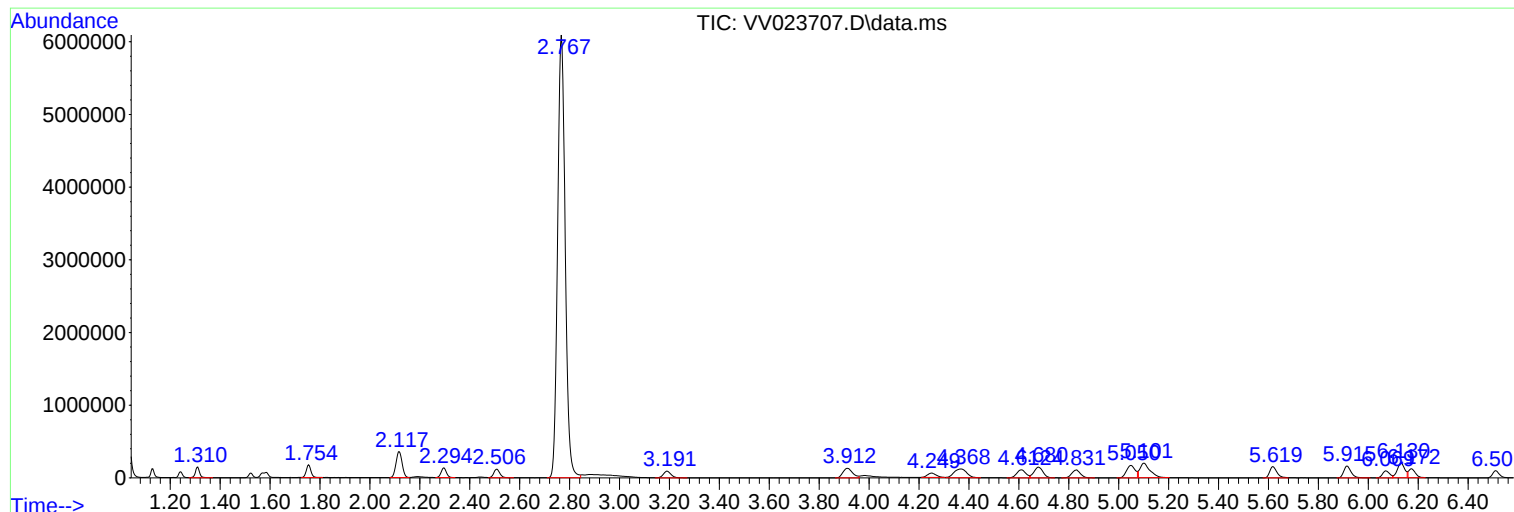

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023707.D
Acq On : 24 Nov 2021 17:51
Operator : SY/MD
Sample : M4821-09MS
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4657MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
Data File : VV023707.D
Acq On : 24 Nov 2021 17:51
Operator : SY/MD
Sample : M4821-09MS
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4657MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc