
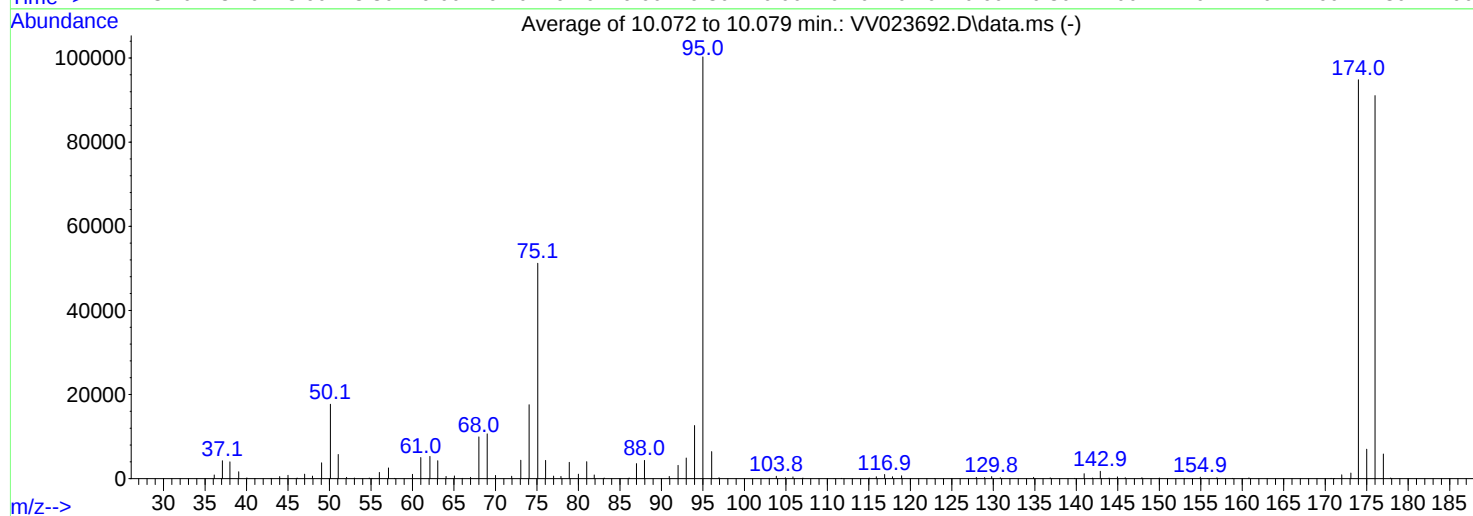


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112421\
 Data File : VV023692.D
 Acq On : 24 Nov 2021 09:30
 Operator : SY/MD
 Sample : BFB240
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB240

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 26 01:51:50 2021

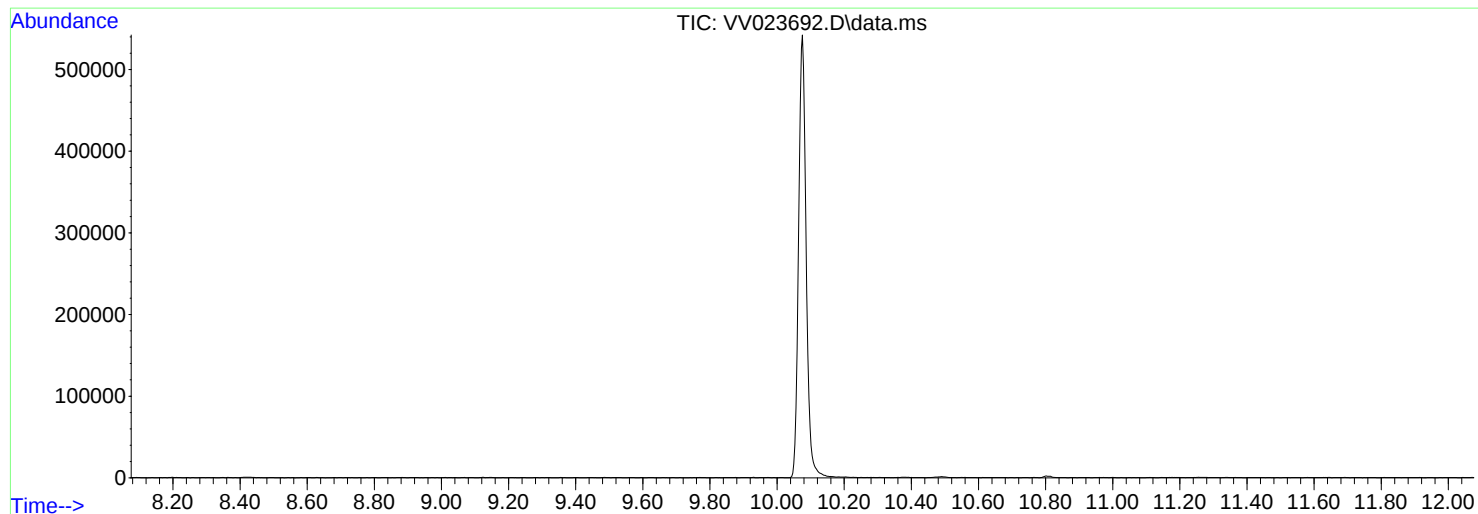

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	17672	PASS
75	95	30	80	51.1	51205	PASS
95	95	100	100	100.0	100285	PASS
96	95	5	9	6.4	6428	PASS
173	174	0.00	2	1.4	1325	PASS
174	95	50	120	94.6	94829	PASS
175	174	5	9	7.4	6984	PASS
176	174	95	105	96.0	91069	PASS
177	176	5	10	6.4	5845	PASS

m/z	Abundance
36.10	800.0
37.10	3825.0
38.00	3841.0
39.00	1508.0
40.00	154.0
41.00	109.0
44.00	635.0
45.00	739.0
46.10	139.0
47.00	911.0
48.00	527.0
49.10	3577.0
50.10	16568.0
51.10	5349.0
52.10	269.0
53.00	136.0
54.80	240.0
56.00	1326.0
57.10	2448.0
57.80	138.0
60.00	1005.0
61.00	4714.0
62.10	4927.0
63.00	3979.0
64.10	526.0
65.00	688.0
67.00	288.0
68.00	9354.0
69.00	10156.0
70.00	724.0
72.00	586.0
73.00	4178.0
74.10	16520.0
75.10	48704.0
76.00	4246.0
77.00	666.0
77.90	433.0
78.90	3664.0
80.00	999.0
81.00	3865.0
81.90	895.0
83.10	186.0
86.20	134.0
87.00	3466.0
87.90	4389.0
90.90	531.0
92.00	2984.0
93.00	4525.0
94.00	12139.0
95.00	95376.0
96.00	6075.0
97.00	190.0
103.00	125.0
103.80	538.0
104.90	246.0
105.90	436.0
107.00	137.0
115.10	119.0
115.90	518.0
116.90	911.0
117.80	449.0
118.90	666.0
127.90	281.0
129.00	285.0
129.80	444.0
130.80	222.0
134.80	321.0
136.90	217.0
140.90	1071.0
141.90	143.0
142.90	1507.0
143.90	160.0
144.90	379.0
145.90	206.0
147.90	308.0
150.00	106.0
153.00	127.0
154.90	326.0
156.90	223.0
158.80	124.0
160.80	247.0
170.70	189.0
171.10	157.0
172.00	894.0
173.10	1319.0
174.00	92776.0
175.00	6816.0
176.00	88568.0
177.00	5643.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
44.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
36.10	938.0
37.10	4535.0
38.00	3998.0
39.10	1739.0
40.10	188.0
42.90	103.0
44.00	705.0
45.00	810.0
46.10	146.0
47.00	1222.0
47.90	622.0
49.00	3914.0
50.10	18184.0
51.00	5918.0
52.00	341.0
53.00	144.0
55.10	223.0
56.00	1555.0
57.10	2604.0
60.00	984.0
61.00	5141.0
62.10	5394.0
63.10	4388.0
64.00	545.0
65.10	634.0
66.00	166.0
67.00	367.0
68.00	10185.0
69.00	10675.0
70.00	817.0
71.90	551.0
73.10	4496.0
74.00	18008.0
75.10	52008.0
76.10	4312.0
77.00	574.0
77.90	595.0
78.90	3932.0
80.00	1056.0
81.00	4062.0
81.90	833.0
83.10	131.0
86.00	139.0
87.00	3640.0
88.00	4066.0
91.00	506.0
92.00	3252.0
93.00	5127.0
94.00	12695.0
95.00	101704.0
96.10	6566.0
96.90	238.0
103.90	587.0
105.00	175.0
105.80	387.0
107.10	169.0
110.80	105.0
111.70	119.0
115.00	189.0
115.90	365.0
116.90	978.0
117.90	478.0
119.00	717.0
128.00	330.0
128.90	242.0
129.80	516.0
130.90	239.0
134.80	293.0
136.80	192.0
139.80	105.0
141.00	1269.0
142.00	196.0
142.90	1911.0
144.00	151.0
144.90	449.0
145.90	251.0
147.90	202.0
150.00	164.0
155.00	385.0
157.00	239.0
160.80	127.0
172.00	919.0
173.10	1264.0
174.00	93144.0
175.00	6887.0
176.00	90256.0
177.00	5795.0
177.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
36.10	893.0
37.10	4423.0
38.00	4182.0
39.10	1695.0
40.00	185.0
43.00	107.0
44.00	676.0
45.00	825.0
46.10	146.0
47.00	1100.0
47.90	636.0
49.00	3870.0
50.10	18264.0
51.00	5975.0
52.00	301.0
53.00	144.0
54.80	235.0
56.00	1536.0
57.10	2655.0
57.90	107.0
60.00	1057.0
61.00	5232.0
62.10	5576.0
63.00	4393.0
64.10	575.0
65.00	679.0
66.00	109.0
67.00	293.0
68.00	10293.0
69.00	11126.0
70.00	802.0
71.90	574.0
73.10	4488.0
74.00	18176.0
75.10	52904.0
76.10	4467.0
77.00	633.0
77.90	566.0
78.90	4015.0
80.00	1096.0
81.00	4162.0
81.90	893.0
83.10	181.0
86.10	136.0
87.00	3663.0
88.00	4564.0
90.90	576.0
92.00	3243.0
93.00	5047.0
94.00	13106.0
95.00	103776.0
96.10	6642.0
97.00	219.0
103.00	111.0
103.80	607.0
104.90	224.0
105.80	398.0
107.00	184.0
111.70	113.0
115.10	156.0
115.90	470.0
116.90	1037.0
117.90	481.0
119.00	739.0
122.90	101.0
128.00	317.0
129.00	305.0
129.80	521.0
130.80	238.0
134.90	335.0
136.80	224.0
139.80	108.0
140.90	1175.0
141.90	175.0
142.90	1829.0
143.90	169.0
145.00	431.0
145.90	243.0
147.90	233.0
150.00	142.0
153.00	107.0
154.90	377.0
155.80	114.0
156.90	266.0
158.80	128.0
160.80	202.0
172.00	938.0
173.10	1393.0
174.00	98568.0
175.00	7250.0
176.00	94384.0
177.00	6096.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

177.90

171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240