

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033064.D
 Acq On : 24 Nov 2023 10:46
 Operator : SY/MD
 Sample : VV1124MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	92	rVB	100509	107763	10.95%	1.366%
2	1.532	146	153	164	rVB	77358	91112	9.26%	1.155%
3	2.060	306	317	336	rBV	163547	241990	24.58%	3.067%
4	2.198	358	360	363	rBV2	411	215	0.02%	0.003%
5	2.240	365	373	383	rBV2	1836	2731	0.28%	0.035%
6	2.487	447	450	454	rVB	310	234	0.02%	0.003%
7	2.510	454	457	460	rBV	377	207	0.02%	0.003%
8	2.671	503	507	510	rBV	313	272	0.03%	0.003%
9	2.696	510	515	522	rVV5	1150	1615	0.16%	0.020%
10	2.728	522	525	529	rVB2	462	390	0.04%	0.005%
11	3.056	625	627	630	rBV	454	252	0.03%	0.003%
12	3.175	659	664	668	rBV	413	426	0.04%	0.005%
13	3.204	670	673	676	rVB2	364	278	0.03%	0.004%
14	3.220	676	678	682	rBV	355	271	0.03%	0.003%
15	3.275	689	695	696	rBV	394	362	0.04%	0.005%
16	3.349	713	718	721	rBV	502	405	0.04%	0.005%
17	3.423	739	741	744	rBV	268	209	0.02%	0.003%
18	3.581	787	790	792	rBV2	345	211	0.02%	0.003%
19	3.780	843	852	883	rBV	56411	153363	15.58%	1.944%
20	4.117	952	957	962	rBV4	448	657	0.07%	0.008%
21	4.246	979	997	1027	rVV2	158804	404958	41.14%	5.133%
22	4.555	1090	1093	1095	rBV2	372	257	0.03%	0.003%
23	4.574	1095	1099	1101	rBV2	405	364	0.04%	0.005%
24	4.622	1111	1114	1116	rBV2	419	250	0.03%	0.003%
25	4.722	1143	1145	1147	rBV2	383	199	0.02%	0.003%
26	4.773	1158	1161	1164	rBV2	434	368	0.04%	0.005%
27	4.815	1169	1174	1177	rBV2	221	241	0.02%	0.003%
28	4.953	1199	1217	1245	rBV3	352470	934655	94.95%	11.846%
29	5.416	1359	1361	1365	rVB2	742	453	0.05%	0.006%
30	5.439	1366	1368	1375	rVB4	651	524	0.05%	0.007%
31	5.471	1375	1378	1380	rBV3	360	218	0.02%	0.003%
32	5.532	1384	1397	1423	rBV	347374	715278	72.66%	9.066%
33	5.825	1478	1488	1508	rVB5	14887	33075	3.36%	0.419%
34	5.986	1525	1538	1562	rBV	200220	409894	41.64%	5.195%
35	6.275	1624	1628	1631	rBV2	390	322	0.03%	0.004%
36	6.307	1636	1638	1641	rVB2	354	231	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033064.D
 Acq On : 24 Nov 2023 10:46
 Operator : SY/MD
 Sample : VV1124MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.680	1751	1754	1758	rBV2	528	416	0.04%	0.005%
38	6.751	1770	1776	1777	rBV	354	299	0.03%	0.004%
39	6.793	1785	1789	1790	rBV2	388	246	0.02%	0.003%
40	6.809	1790	1794	1798	rVB3	365	344	0.03%	0.004%
41	6.912	1815	1826	1851	rBV	115736	217226	22.07%	2.753%
42	7.105	1883	1886	1890	rVB3	630	503	0.05%	0.006%
43	7.243	1917	1929	1956	rBV	431188	757119	76.91%	9.596%
44	7.551	2016	2025	2042	rBV	83059	147903	15.03%	1.875%
45	7.715	2074	2076	2078	rBV2	501	229	0.02%	0.003%
46	7.831	2107	2112	2114	rBV3	639	465	0.05%	0.006%
47	7.969	2151	2155	2160	rVB2	327	342	0.03%	0.004%
48	8.021	2160	2171	2198	rBV	191200	360124	36.58%	4.564%
49	8.471	2309	2311	2314	rBV2	401	235	0.02%	0.003%
50	8.503	2320	2321	2325	rVB	549	248	0.03%	0.003%
51	8.532	2325	2330	2333	rVB2	429	422	0.04%	0.005%
52	8.603	2348	2352	2354	rBV2	280	197	0.02%	0.002%
53	8.616	2354	2356	2358	rBV2	512	279	0.03%	0.004%
54	8.686	2375	2378	2381	rBV2	228	199	0.02%	0.003%
55	8.725	2387	2390	2395	rVB	372	234	0.02%	0.003%
56	8.783	2395	2408	2440	rBV	564903	915141	92.97%	11.599%
57	9.085	2500	2502	2506	rVB4	516	313	0.03%	0.004%
58	9.162	2522	2526	2528	rBV2	323	236	0.02%	0.003%
59	9.204	2537	2539	2541	rBV	374	209	0.02%	0.003%
60	9.249	2546	2553	2556	rBV3	370	471	0.05%	0.006%
61	9.426	2604	2608	2613	rBV2	561	396	0.04%	0.005%
62	9.465	2617	2620	2623	rBV2	359	231	0.02%	0.003%
63	9.487	2623	2627	2629	rBV2	764	653	0.07%	0.008%
64	9.590	2654	2659	2665	rVB	332	295	0.03%	0.004%
65	9.747	2706	2708	2711	rBV2	409	195	0.02%	0.002%
66	9.873	2741	2747	2752	rBV2	944	1200	0.12%	0.015%
67	10.034	2794	2797	2804	rVV2	370	369	0.04%	0.005%
68	10.085	2809	2813	2817	rBV2	337	300	0.03%	0.004%
69	10.104	2817	2819	2821	rVB2	478	198	0.02%	0.003%
70	10.153	2821	2834	2850	rBV	275308	436766	44.37%	5.536%
71	10.326	2878	2888	2896	rBV5	1721	2946	0.30%	0.037%
72	10.384	2902	2906	2909	rBV2	313	298	0.03%	0.004%
73	10.603	2970	2974	2975	rBV	266	225	0.02%	0.003%
74	10.651	2986	2989	2991	rBV2	264	193	0.02%	0.002%
75	10.815	3037	3040	3043	rVB	325	212	0.02%	0.003%
76	10.831	3043	3045	3049	rBV	398	256	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033064.D
 Acq On : 24 Nov 2023 10:46
 Operator : SY/MD
 Sample : VV1124MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.857	3049	3053	3055	rBV3	1324	1087	0.11%	0.014%
78	10.950	3078	3082	3085	rVB2	397	334	0.03%	0.004%
79	10.979	3085	3091	3093	rBV	531	456	0.05%	0.006%
80	11.130	3130	3138	3144	rBV5	2667	3966	0.40%	0.050%
81	11.185	3144	3155	3178	rBV	649885	984371	100.00%	12.476%
82	11.561	3260	3272	3293	rBV	529774	844226	85.76%	10.700%
83	11.828	3352	3355	3360	rBV2	636	532	0.05%	0.007%
84	11.931	3384	3387	3392	rBV2	338	263	0.03%	0.003%
85	12.198	3463	3470	3477	rVB6	1684	2483	0.25%	0.031%
86	12.365	3517	3522	3523	rBV2	618	533	0.05%	0.007%
87	12.442	3540	3546	3549	rBV2	392	400	0.04%	0.005%
88	12.484	3554	3559	3562	rBV2	317	311	0.03%	0.004%
89	12.590	3584	3592	3603	rBV3	4621	7388	0.75%	0.094%
90	12.680	3617	3620	3623	rBV3	401	366	0.04%	0.005%
91	12.931	3696	3698	3702	rBV2	257	184	0.02%	0.002%
92	13.117	3752	3756	3758	rBV	340	271	0.03%	0.003%
93	13.201	3774	3782	3796	rVV4	9752	16497	1.68%	0.209%
94	13.445	3849	3858	3874	rBV	32108	50642	5.14%	0.642%
95	13.686	3924	3933	3943	rBV3	14498	21781	2.21%	0.276%
96	13.860	3984	3987	3988	rBV	432	206	0.02%	0.003%
97	13.937	4006	4011	4012	rBV2	539	445	0.05%	0.006%
98	14.152	4076	4078	4080	rBV2	425	225	0.02%	0.003%
99	14.484	4178	4181	4183	rBV	518	245	0.02%	0.003%
100	14.551	4200	4202	4204	rBV	563	236	0.02%	0.003%


Sum of corrected areas: 7889831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033064.D
Acq On : 24 Nov 2023 10:46
Operator : SY/MD
Sample : VV1124MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

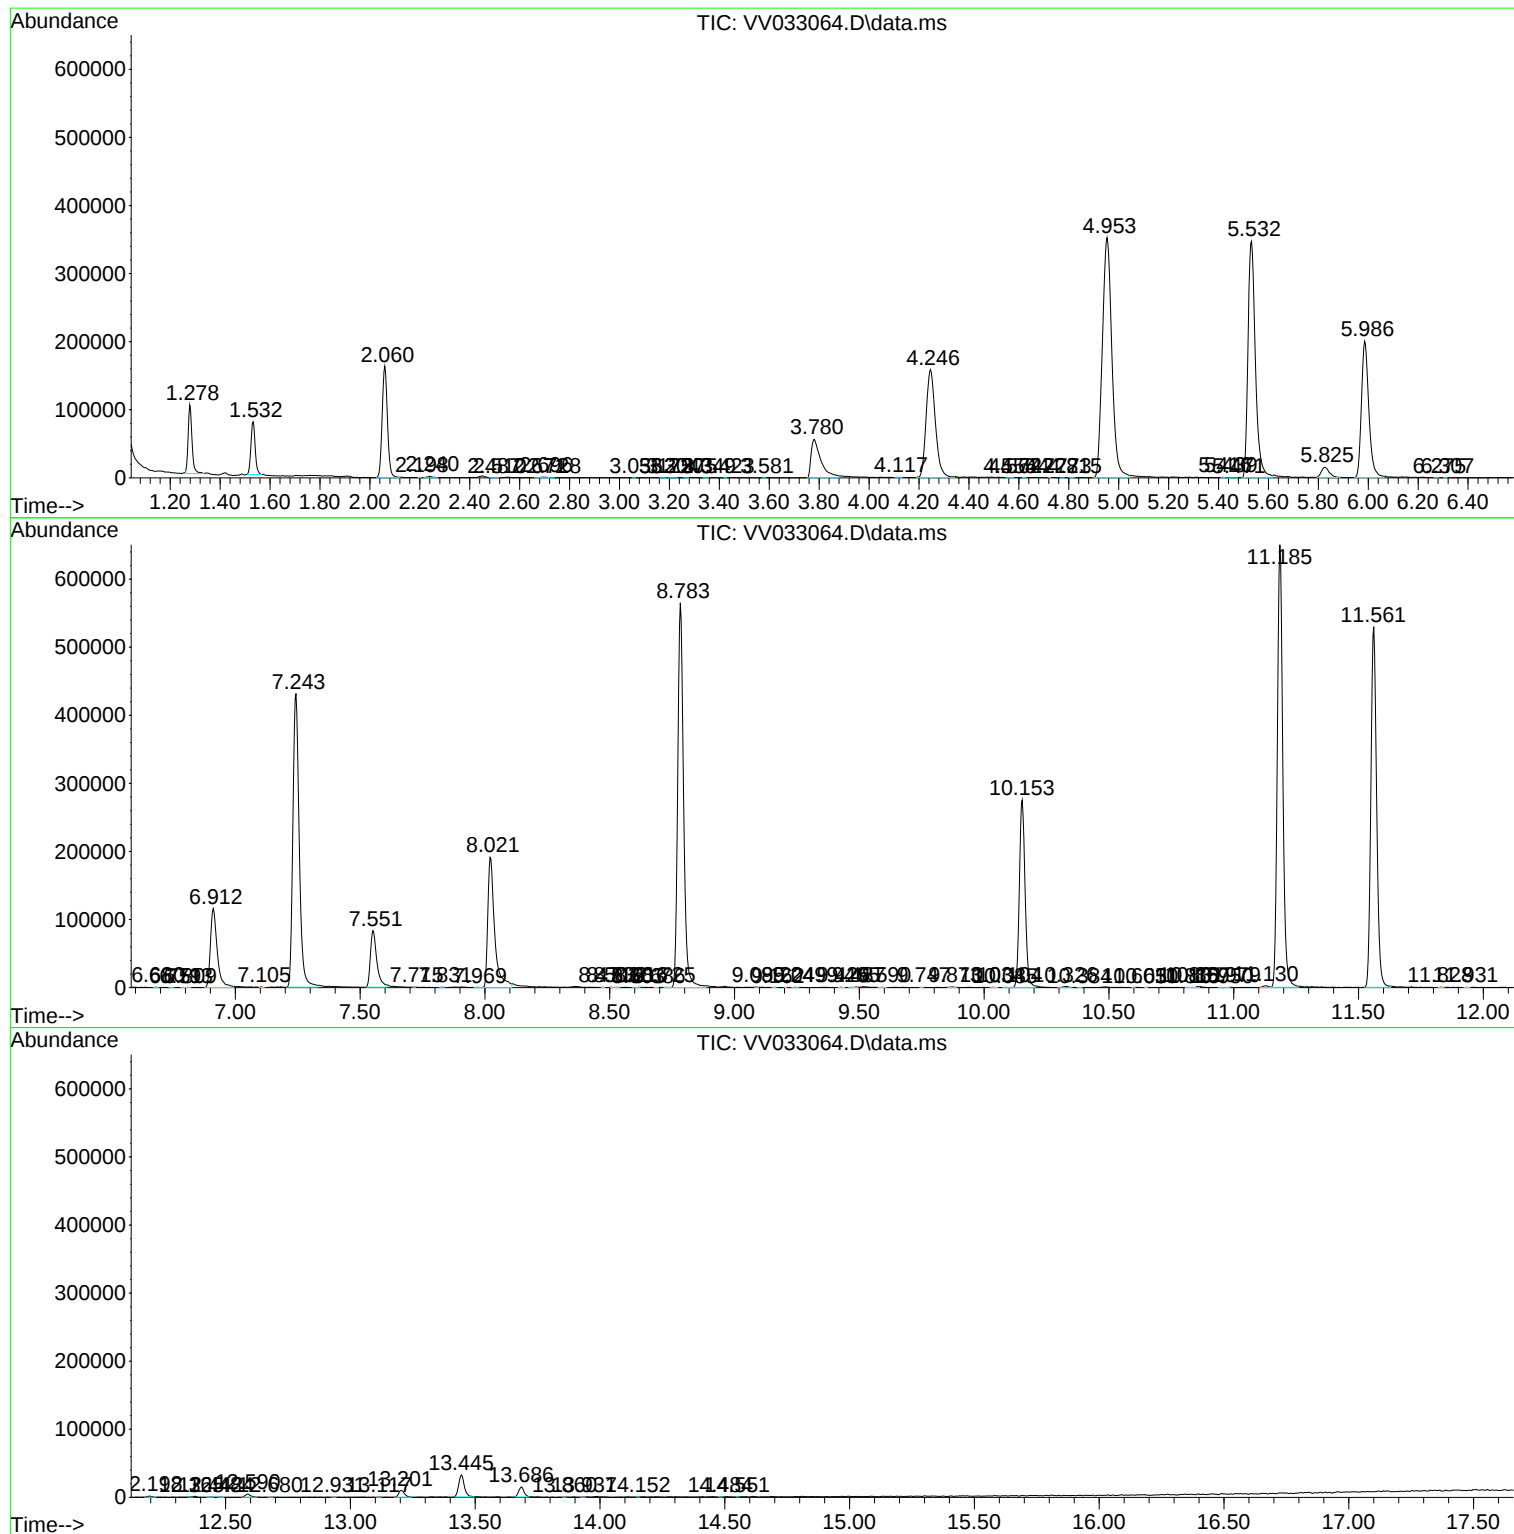

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033064.D
Acq On : 24 Nov 2023 10:46
Operator : SY/MD
Sample : VV1124MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033064.D
Acq On : 24 Nov 2023 10:46
Operator : SY/MD
Sample : VV1124MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------