

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033065.D
 Acq On : 24 Nov 2023 11:09
 Operator : SY/MD
 Sample : VV1124WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	93	rVB	94052	101294	11.10%	1.335%
2	1.532	146	153	169	rVB	75709	91180	9.99%	1.202%
3	1.976	287	291	298	rVB2	683	415	0.05%	0.005%
4	2.060	307	317	331	rBV	156309	228620	25.04%	3.014%
5	2.182	353	355	361	rVB2	547	350	0.04%	0.005%
6	2.240	367	373	380	rBV4	1195	1701	0.19%	0.022%
7	2.314	393	396	398	rBV	394	230	0.03%	0.003%
8	2.452	431	439	448	rVB6	2880	4596	0.50%	0.061%
9	2.555	463	471	476	rBV3	974	1234	0.14%	0.016%
10	2.577	476	478	484	rVB2	584	395	0.04%	0.005%
11	2.764	533	536	540	rVB3	395	286	0.03%	0.004%
12	2.860	559	566	568	rBV3	389	473	0.05%	0.006%
13	2.931	586	588	595	rBV2	295	331	0.04%	0.004%
14	3.124	643	648	650	rVV	218	209	0.02%	0.003%
15	3.253	682	688	691	rBV	552	458	0.05%	0.006%
16	3.349	712	718	723	rBV2	383	584	0.06%	0.008%
17	3.510	763	768	770	rBV2	246	177	0.02%	0.002%
18	3.574	782	788	789	rBV2	354	291	0.03%	0.004%
19	3.693	821	825	827	rVB	345	262	0.03%	0.003%
20	3.716	828	832	835	rBV	273	246	0.03%	0.003%
21	3.783	844	853	882	rBV2	58817	159413	17.46%	2.102%
22	4.021	923	927	930	rBV3	541	529	0.06%	0.007%
23	4.108	951	954	959	rBV3	436	470	0.05%	0.006%
24	4.249	980	998	1030	rBV2	153927	397363	43.53%	5.239%
25	4.645	1119	1121	1124	rBV2	365	287	0.03%	0.004%
26	4.706	1139	1140	1144	rBV2	364	235	0.03%	0.003%
27	4.732	1144	1148	1150	rBV2	304	262	0.03%	0.003%
28	4.789	1162	1166	1167	rBV2	296	194	0.02%	0.003%
29	4.854	1181	1186	1189	rBV3	492	399	0.04%	0.005%
30	4.957	1201	1218	1248	rBV2	336553	906013	99.24%	11.945%
31	5.333	1333	1335	1338	rBV3	408	248	0.03%	0.003%
32	5.484	1378	1382	1384	rBV	295	244	0.03%	0.003%
33	5.535	1385	1398	1424	rBV	321670	663895	72.72%	8.753%
34	5.828	1479	1489	1507	rBV4	13889	30285	3.32%	0.399%
35	5.989	1526	1539	1564	rBV	196346	408513	44.75%	5.386%
36	6.195	1601	1603	1607	rBV3	543	432	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033065.D
 Acq On : 24 Nov 2023 11:09
 Operator : SY/MD
 Sample : VV1124WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.249	1617	1620	1621	rBV2	456	225	0.02%	0.003%
38	6.317	1639	1641	1643	rBV	386	201	0.02%	0.003%
39	6.381	1657	1661	1663	rBV3	407	310	0.03%	0.004%
40	6.680	1752	1754	1757	rVB	425	209	0.02%	0.003%
41	6.741	1770	1773	1774	rBV	466	275	0.03%	0.004%
42	6.783	1780	1786	1788	rVB2	389	382	0.04%	0.005%
43	6.860	1808	1810	1813	rBV	383	263	0.03%	0.003%
44	6.915	1816	1827	1854	rBV	111726	212028	23.23%	2.795%
45	7.191	1911	1913	1916	rBV4	467	360	0.04%	0.005%
46	7.243	1918	1929	1961	rVV	417825	740905	81.16%	9.768%
47	7.555	2016	2026	2048	rBV	81560	148252	16.24%	1.955%
48	7.741	2082	2084	2090	rBV4	522	479	0.05%	0.006%
49	7.876	2120	2126	2128	rBV2	572	534	0.06%	0.007%
50	7.915	2136	2138	2139	rBV	437	214	0.02%	0.003%
51	7.982	2155	2159	2162	rBV2	222	192	0.02%	0.003%
52	8.024	2162	2172	2207	rBV	204752	391238	42.86%	5.158%
53	8.439	2299	2301	2304	rVB2	421	187	0.02%	0.002%
54	8.455	2304	2306	2309	rBV3	263	191	0.02%	0.003%
55	8.484	2313	2315	2317	rBV	355	184	0.02%	0.002%
56	8.722	2386	2389	2395	rBV2	326	302	0.03%	0.004%
57	8.783	2397	2408	2435	rBV	513902	851795	93.30%	11.230%
58	9.223	2542	2545	2549	rBV	435	277	0.03%	0.004%
59	9.362	2585	2588	2592	rVB3	345	228	0.02%	0.003%
60	9.381	2592	2594	2600	rVB2	324	203	0.02%	0.003%
61	9.497	2625	2630	2631	rBV2	523	456	0.05%	0.006%
62	9.725	2696	2701	2702	rBV	566	419	0.05%	0.006%
63	9.764	2708	2713	2717	rBV2	238	233	0.03%	0.003%
64	9.857	2740	2742	2745	rBV	404	291	0.03%	0.004%
65	9.928	2761	2764	2766	rBV2	388	199	0.02%	0.003%
66	9.940	2766	2768	2770	rBV	304	176	0.02%	0.002%
67	10.153	2822	2834	2857	rBV	285915	449453	49.23%	5.925%
68	10.323	2881	2887	2899	rBV5	1562	2631	0.29%	0.035%
69	10.590	2966	2970	2973	rBV	308	221	0.02%	0.003%
70	10.770	3024	3026	3029	rBV2	341	200	0.02%	0.003%
71	10.985	3090	3093	3096	rVB	265	177	0.02%	0.002%
72	11.127	3130	3137	3144	rBV6	1431	2043	0.22%	0.027%
73	11.185	3144	3155	3178	rBV	582859	912928	100.00%	12.036%
74	11.419	3226	3228	3231	rBV2	421	279	0.03%	0.004%
75	11.561	3260	3272	3296	rBV	525836	829774	90.89%	10.939%
76	11.982	3401	3403	3406	rBV2	583	321	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033065.D
 Acq On : 24 Nov 2023 11:09
 Operator : SY/MD
 Sample : VV1124WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	12.201	3464	3471	3481	rVB4	2490	3879	0.42%	0.051%
78	12.288	3494	3498	3500	rBV2	392	202	0.02%	0.003%
79	12.310	3500	3505	3510	rBV2	323	475	0.05%	0.006%
80	12.487	3557	3560	3562	rVB2	512	272	0.03%	0.004%
81	12.519	3566	3570	3572	rBV2	230	205	0.02%	0.003%
82	12.590	3583	3592	3601	rBV6	1347	2453	0.27%	0.032%
83	12.779	3649	3651	3653	rBV	360	182	0.02%	0.002%
84	12.824	3659	3665	3669	rBV2	374	451	0.05%	0.006%
85	12.921	3692	3695	3698	rVB	336	232	0.03%	0.003%
86	12.953	3702	3705	3706	rBV2	364	207	0.02%	0.003%
87	13.104	3749	3752	3755	rBV2	374	281	0.03%	0.004%
88	13.152	3765	3767	3776	rVB3	451	548	0.06%	0.007%
89	13.204	3777	3783	3796	rVB6	2739	4423	0.48%	0.058%
90	13.448	3852	3859	3869	rVB	7629	11046	1.21%	0.146%
91	13.615	3909	3911	3914	rBV	374	219	0.02%	0.003%
92	13.635	3914	3917	3919	rBV2	464	316	0.03%	0.004%
93	13.686	3926	3933	3945	rBV5	3545	5511	0.60%	0.073%
94	13.831	3975	3978	3979	rBV	509	261	0.03%	0.003%
95	13.931	4006	4009	4010	rBV2	561	307	0.03%	0.004%
96	14.027	4036	4039	4042	rBV3	979	789	0.09%	0.010%
97	14.056	4046	4048	4052	rVV2	497	367	0.04%	0.005%
98	14.072	4052	4053	4058	rBV3	439	342	0.04%	0.005%
99	14.728	4255	4257	4260	rBV	620	431	0.05%	0.006%
100	14.889	4305	4307	4309	rBV	780	383	0.04%	0.005%


Sum of corrected areas: 7585131

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033065.D
Acq On : 24 Nov 2023 11:09
Operator : SY/MD
Sample : VV1124WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

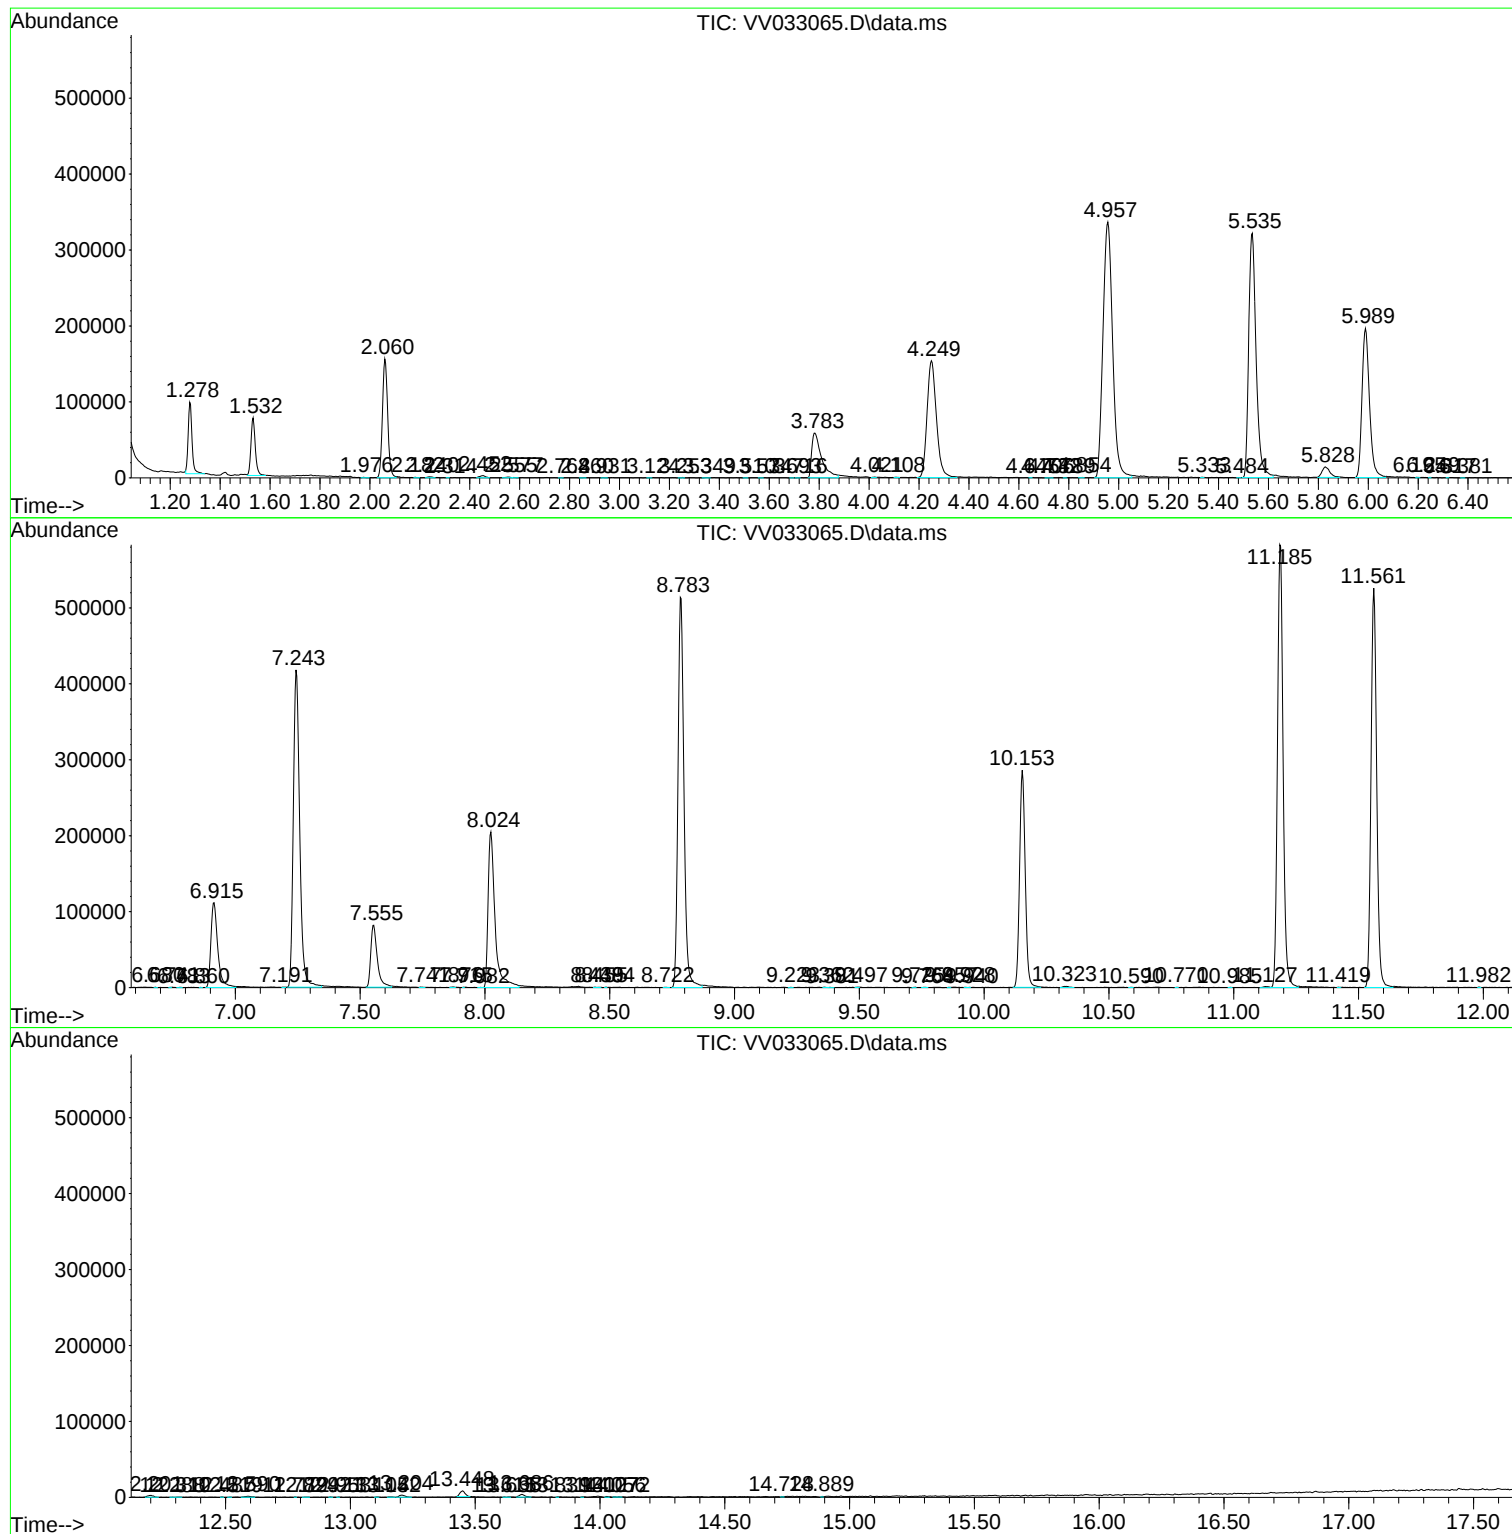

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033065.D
Acq On : 24 Nov 2023 11:09
Operator : SY/MD
Sample : VV1124WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033065.D
Acq On : 24 Nov 2023 11:09
Operator : SY/MD
Sample : VV1124WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------