

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112423\
 Data File : VW033067.D
 Acq On : 24 Nov 2023 12:24
 Operator : SY/MD
 Sample : 05497-02ME
 Misc : 2.09G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VW033067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	86851	121034	10.55%	1.478%
2	2.040	301	311	330	rVB	153610	227321	19.82%	2.777%
3	2.111	330	333	336	rBV2	655	520	0.05%	0.006%
4	2.220	365	367	375	rVB2	802	837	0.07%	0.010%
5	2.359	407	410	411	rBV	589	263	0.02%	0.003%
6	2.372	411	414	416	rVV	396	279	0.02%	0.003%
7	2.436	425	434	444	rBV3	6292	10959	0.96%	0.134%
8	2.552	459	470	489	rBV3	4316	9832	0.86%	0.120%
9	2.693	511	514	517	rBV3	742	530	0.05%	0.006%
10	2.950	591	594	596	rBV3	425	269	0.02%	0.003%
11	3.150	652	656	660	rVV	265	208	0.02%	0.003%
12	3.201	669	672	678	rVB	401	365	0.03%	0.004%
13	3.272	691	694	697	rBV	428	270	0.02%	0.003%
14	3.532	772	775	777	rVB	538	223	0.02%	0.003%
15	3.574	786	788	792	rVB	389	279	0.02%	0.003%
16	3.606	792	798	799	rBV	360	278	0.02%	0.003%
17	3.764	842	847	848	rBV2	347	256	0.02%	0.003%
18	3.793	848	856	886	rBV2	40672	139776	12.19%	1.707%
19	4.188	976	979	980	rBV	376	230	0.02%	0.003%
20	4.243	980	996	1023	rVV2	152916	412901	36.00%	5.044%
21	4.638	1115	1119	1120	rBV2	367	285	0.02%	0.003%
22	4.654	1123	1124	1128	rVB	518	218	0.02%	0.003%
23	4.677	1128	1131	1134	rBV2	420	336	0.03%	0.004%
24	4.722	1142	1145	1147	rBV	357	211	0.02%	0.003%
25	4.828	1175	1178	1181	rBV	397	240	0.02%	0.003%
26	4.947	1200	1215	1242	rBV2	357020	930528	81.12%	11.367%
27	5.249	1306	1309	1311	rBV3	610	399	0.03%	0.005%
28	5.365	1341	1345	1348	rVB2	378	223	0.02%	0.003%
29	5.404	1353	1357	1359	rBV2	409	312	0.03%	0.004%
30	5.420	1359	1362	1364	rBV2	531	317	0.03%	0.004%
31	5.529	1385	1396	1425	rBV	377166	802940	70.00%	9.808%
32	5.825	1478	1488	1502	rBV3	14478	30944	2.70%	0.378%
33	5.986	1526	1538	1563	rBV	195284	413702	36.07%	5.053%
34	6.326	1640	1644	1646	rBV2	319	232	0.02%	0.003%
35	6.346	1646	1650	1653	rVV	220	253	0.02%	0.003%
36	6.439	1677	1679	1686	rVB2	467	382	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033067.D
 Acq On : 24 Nov 2023 12:24
 Operator : SY/MD
 Sample : 05497-02ME
 Misc : 2.09G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.468	1686	1688	1692	rBV	300	278	0.02%	0.003%
38	6.503	1698	1699	1704	rBV	358	246	0.02%	0.003%
39	6.584	1718	1724	1725	rBV2	542	413	0.04%	0.005%
40	6.629	1736	1738	1741	rVB2	527	308	0.03%	0.004%
41	6.651	1742	1745	1748	rBV2	468	371	0.03%	0.005%
42	6.699	1757	1760	1761	rBV3	357	199	0.02%	0.002%
43	6.912	1815	1826	1846	rBV	117663	234197	20.42%	2.861%
44	7.130	1891	1894	1896	rBV2	637	437	0.04%	0.005%
45	7.169	1903	1906	1913	rBV2	654	573	0.05%	0.007%
46	7.243	1917	1929	1961	rBV	406699	738497	64.38%	9.021%
47	7.471	1998	2000	2004	rVB3	541	304	0.03%	0.004%
48	7.555	2015	2026	2057	rBV	80104	164588	14.35%	2.010%
49	7.741	2080	2084	2086	rBV	553	404	0.04%	0.005%
50	7.789	2097	2099	2102	rVB2	418	213	0.02%	0.003%
51	7.834	2110	2113	2115	rBV2	338	252	0.02%	0.003%
52	7.854	2115	2119	2120	rBV	402	240	0.02%	0.003%
53	8.047	2166	2179	2217	rBV3	129599	378085	32.96%	4.618%
54	8.465	2307	2309	2312	rBV3	433	254	0.02%	0.003%
55	8.548	2333	2335	2337	rVV	333	205	0.02%	0.003%
56	8.564	2337	2340	2342	rVV	442	273	0.02%	0.003%
57	8.583	2342	2346	2348	rVV3	547	397	0.03%	0.005%
58	8.786	2393	2409	2436	rBV	588344	1039775	90.65%	12.701%
59	8.976	2466	2468	2472	rBV3	519	332	0.03%	0.004%
60	9.034	2484	2486	2489	rVB2	696	429	0.04%	0.005%
61	9.169	2524	2528	2532	rBV	234	258	0.02%	0.003%
62	9.313	2568	2573	2575	rVB2	305	237	0.02%	0.003%
63	9.374	2588	2592	2594	rVB2	514	357	0.03%	0.004%
64	9.436	2606	2611	2613	rBV2	285	290	0.03%	0.004%
65	9.603	2657	2663	2668	rVV2	468	627	0.05%	0.008%
66	9.780	2716	2718	2722	rBV	279	213	0.02%	0.003%
67	9.963	2772	2775	2778	rVB2	470	249	0.02%	0.003%
68	10.159	2824	2836	2855	rBV	282187	469576	40.94%	5.736%
69	10.317	2882	2885	2886	rBV	568	329	0.03%	0.004%
70	10.445	2921	2925	2930	rVB2	368	315	0.03%	0.004%
71	10.471	2930	2933	2935	rBV	336	203	0.02%	0.002%
72	10.593	2968	2971	2978	rVB3	374	353	0.03%	0.004%
73	10.722	3006	3011	3013	rBV3	263	246	0.02%	0.003%
74	10.776	3024	3028	3030	rBV2	430	297	0.03%	0.004%
75	10.911	3067	3070	3072	rBV	268	205	0.02%	0.003%
76	10.924	3072	3074	3078	rVB2	514	363	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112423\
 Data File : VW033067.D
 Acq On : 24 Nov 2023 12:24
 Operator : SY/MD
 Sample : 05497-02ME
 Misc : 2.09G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.944	3078	3080	3083	rBV2	379	267	0.02%	0.003%
78	11.143	3138	3142	3144	rBV2	516	419	0.04%	0.005%
79	11.188	3145	3156	3184	rVV	743903	1147050	100.00%	14.012%
80	11.410	3222	3225	3229	rBV3	571	433	0.04%	0.005%
81	11.564	3260	3273	3290	rBV	563249	887233	77.35%	10.838%
82	11.841	3357	3359	3362	rVB3	505	229	0.02%	0.003%
83	12.194	3465	3469	3470	rBV2	773	555	0.05%	0.007%
84	12.239	3481	3483	3488	rVB	533	290	0.03%	0.004%
85	12.596	3591	3594	3595	rBV2	524	205	0.02%	0.003%
86	12.696	3621	3625	3628	rBV	474	413	0.04%	0.005%
87	12.828	3663	3666	3668	rBV2	303	234	0.02%	0.003%
88	12.940	3698	3701	3707	rBV3	543	505	0.04%	0.006%
89	13.214	3781	3786	3789	rBV3	932	1073	0.09%	0.013%
90	13.294	3808	3811	3818	rBV4	440	518	0.05%	0.006%
91	13.426	3846	3852	3853	rBV2	773	569	0.05%	0.007%
92	13.554	3890	3892	3899	rVB3	479	351	0.03%	0.004%
93	13.583	3899	3901	3905	rBV2	393	270	0.02%	0.003%
94	13.644	3916	3920	3924	rBV3	429	328	0.03%	0.004%
95	13.667	3925	3927	3929	rBV	478	263	0.02%	0.003%
96	13.763	3954	3957	3961	rBV2	415	315	0.03%	0.004%
97	14.259	4109	4111	4114	rBV4	522	312	0.03%	0.004%
98	14.313	4125	4128	4129	rBV2	528	304	0.03%	0.004%
99	14.464	4173	4175	4178	rBV2	442	297	0.03%	0.004%
100	15.088	4368	4369	4373	rBV4	729	488	0.04%	0.006%




Sum of corrected areas: 8186461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033067.D
Acq On : 24 Nov 2023 12:24
Operator : SY/MD
Sample : 05497-02ME
Misc : 2.09G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

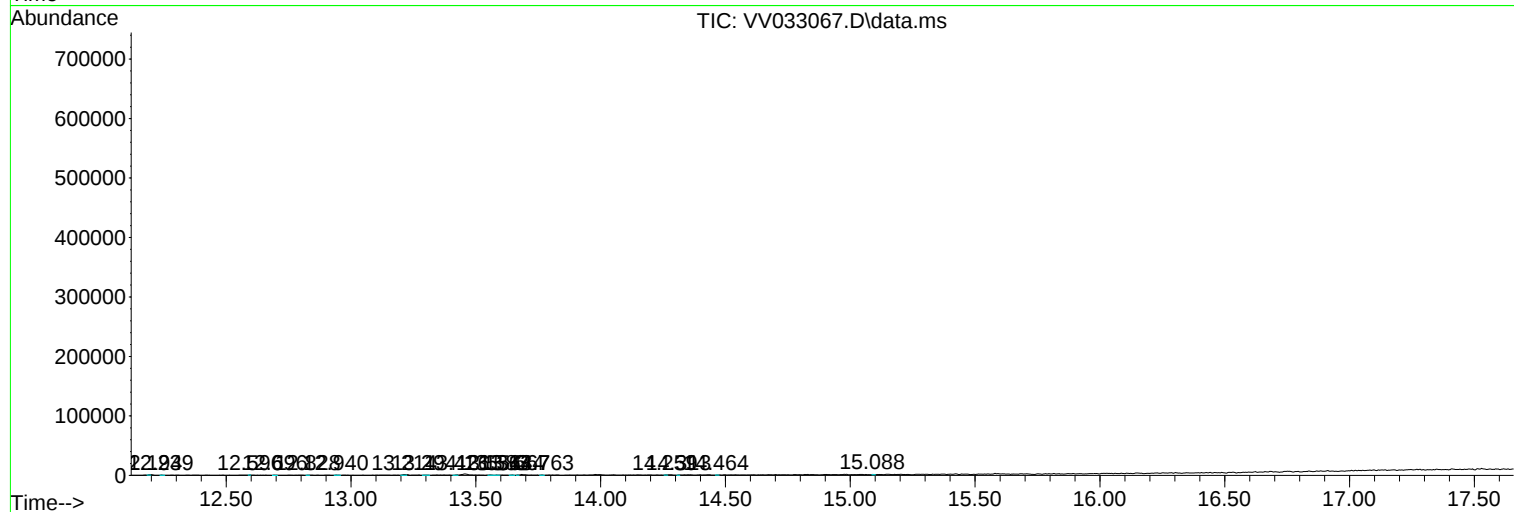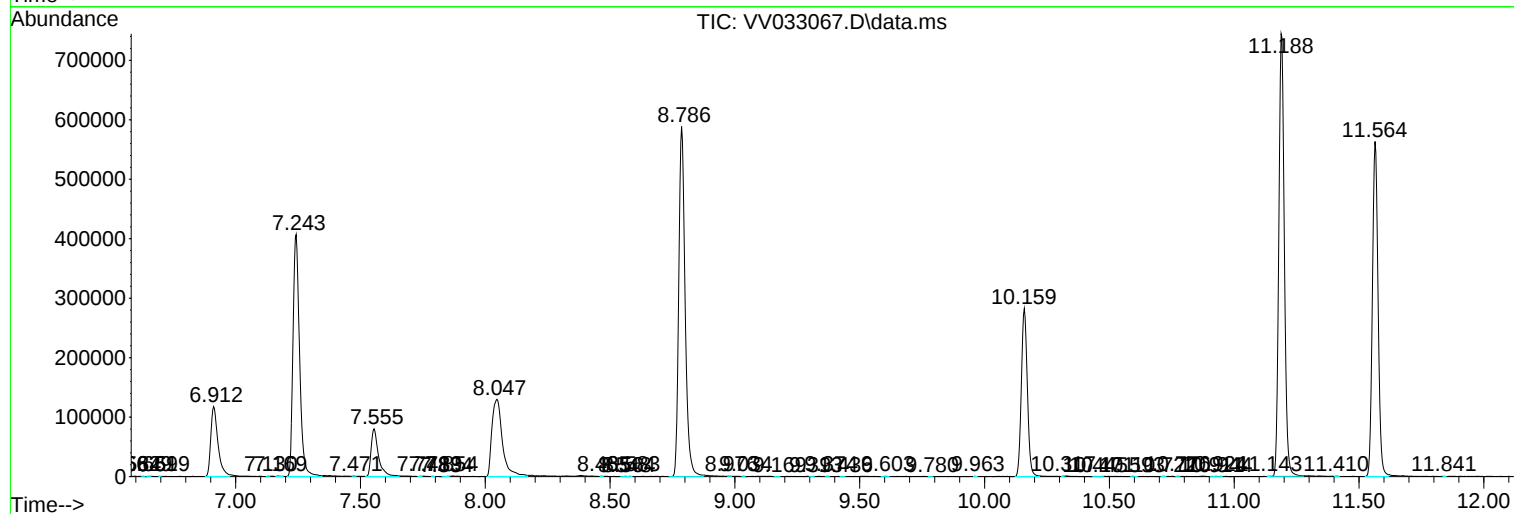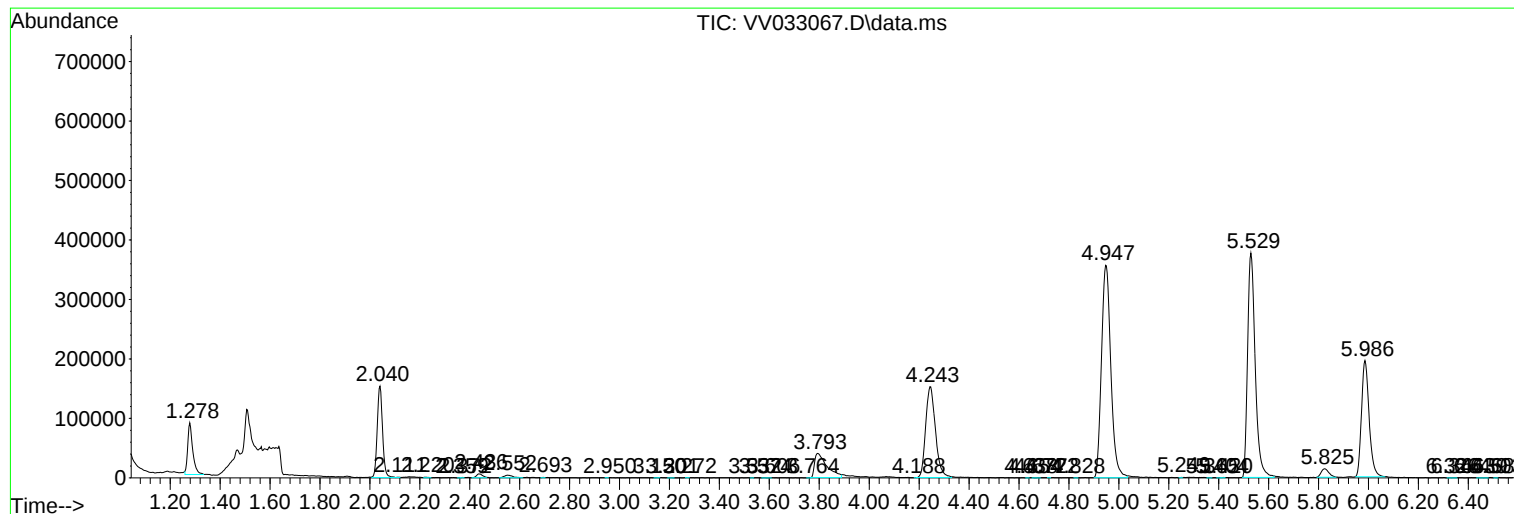

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033067.D
Acq On : 24 Nov 2023 12:24
Operator : SY/MD
Sample : 05497-02ME
Misc : 2.09G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033067.D
Acq On : 24 Nov 2023 12:24
Operator : SY/MD
Sample : 05497-02ME
Misc : 2.09G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc