

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033069.D
 Acq On : 24 Nov 2023 13:16
 Operator : SY/MD
 Sample : VIBLK258
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	91	rVB	77651	85535	10.33%	1.249%
2	1.532	146	153	165	rVB	63083	76426	9.23%	1.116%
3	2.060	307	317	334	rBV	129584	192924	23.30%	2.818%
4	2.169	348	351	353	rVB	418	206	0.02%	0.003%
5	2.192	357	358	362	rVB	321	178	0.02%	0.003%
6	2.217	362	366	367	rBV	325	217	0.03%	0.003%
7	2.320	395	398	402	rVV	529	428	0.05%	0.006%
8	2.356	406	409	413	rVV4	521	322	0.04%	0.005%
9	2.407	423	425	428	rVB	372	171	0.02%	0.002%
10	2.446	428	437	451	rBV5	3084	5568	0.67%	0.081%
11	2.555	464	471	472	rBV2	1189	1321	0.16%	0.019%
12	2.622	490	492	498	rVB2	560	517	0.06%	0.008%
13	2.819	550	553	556	rVV2	283	185	0.02%	0.003%
14	3.140	650	653	654	rBV	361	204	0.02%	0.003%
15	3.211	672	675	677	rVV	286	190	0.02%	0.003%
16	3.227	677	680	683	rVB	255	212	0.03%	0.003%
17	3.243	683	685	687	rBV	412	207	0.02%	0.003%
18	3.256	687	689	693	rVV2	439	297	0.04%	0.004%
19	3.278	693	696	698	rVV2	272	182	0.02%	0.003%
20	3.339	712	715	716	rBV2	283	183	0.02%	0.003%
21	3.384	725	729	735	rVB2	460	418	0.05%	0.006%
22	3.478	754	758	760	rBV	317	263	0.03%	0.004%
23	3.577	784	789	792	rBV	399	338	0.04%	0.005%
24	3.780	842	852	877	rBV	55889	152487	18.41%	2.227%
25	4.246	981	997	1029	rBV	138150	361384	43.64%	5.279%
26	4.529	1081	1085	1087	rBV2	476	350	0.04%	0.005%
27	4.558	1092	1094	1096	rVV3	484	245	0.03%	0.004%
28	4.584	1100	1102	1107	rBV3	410	336	0.04%	0.005%
29	4.690	1128	1135	1137	rBV3	365	440	0.05%	0.006%
30	4.712	1139	1142	1145	rVB2	325	203	0.02%	0.003%
31	4.748	1151	1153	1158	rVB2	545	270	0.03%	0.004%
32	4.953	1202	1217	1247	rBV3	307031	823433	99.44%	12.028%
33	5.413	1356	1360	1362	rBV2	579	456	0.06%	0.007%
34	5.487	1380	1383	1384	rBV	575	311	0.04%	0.005%
35	5.532	1386	1397	1435	rVV	297981	619681	74.83%	9.052%
36	5.831	1481	1490	1502	rVB4	12866	24185	2.92%	0.353%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112423\
 Data File : VW033069.D
 Acq On : 24 Nov 2023 13:16
 Operator : SY/MD
 Sample : VIBLK258
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.989	1525	1539	1566	rBV	180134	374349	45.21%	5.468%
38	6.323	1639	1643	1644	rBV	323	250	0.03%	0.004%
39	6.355	1650	1653	1659	rBV	382	391	0.05%	0.006%
40	6.394	1659	1665	1671	rBV2	557	617	0.07%	0.009%
41	6.461	1683	1686	1691	rBV2	326	312	0.04%	0.005%
42	6.571	1718	1720	1722	rBV	371	245	0.03%	0.004%
43	6.632	1737	1739	1740	rBV	327	160	0.02%	0.002%
44	6.680	1749	1754	1757	rBV2	304	231	0.03%	0.003%
45	6.773	1779	1783	1787	rBV2	442	391	0.05%	0.006%
46	6.912	1816	1826	1846	rBV	104091	191939	23.18%	2.804%
47	7.178	1906	1909	1912	rBV3	387	290	0.04%	0.004%
48	7.243	1917	1929	1963	rBV	366772	651751	78.70%	9.520%
49	7.551	2015	2025	2052	rBV	75955	139152	16.80%	2.033%
50	7.780	2094	2096	2100	rVB2	591	385	0.05%	0.006%
51	7.854	2117	2119	2122	rBV	303	202	0.02%	0.003%
52	7.931	2141	2143	2146	rBV2	305	203	0.02%	0.003%
53	8.024	2163	2172	2210	rVV	189163	361248	43.62%	5.277%
54	8.503	2318	2321	2323	rBV2	292	178	0.02%	0.003%
55	8.600	2347	2351	2354	rBV2	226	171	0.02%	0.002%
56	8.661	2366	2370	2373	rBV3	277	247	0.03%	0.004%
57	8.709	2378	2385	2386	rBV2	243	232	0.03%	0.003%
58	8.786	2397	2409	2428	rBV	489225	786898	95.02%	11.495%
59	9.043	2487	2489	2493	rBV2	254	207	0.02%	0.003%
60	9.455	2614	2617	2619	rBV	462	331	0.04%	0.005%
61	9.584	2654	2657	2660	rBV2	208	187	0.02%	0.003%
62	9.622	2665	2669	2672	rBV2	306	368	0.04%	0.005%
63	9.876	2742	2748	2751	rVB2	380	366	0.04%	0.005%
64	9.899	2751	2755	2758	rBV2	177	185	0.02%	0.003%
65	10.075	2808	2810	2818	rVB2	297	314	0.04%	0.005%
66	10.153	2819	2834	2857	rBV	269456	419499	50.66%	6.128%
67	10.468	2929	2932	2934	rBV	262	182	0.02%	0.003%
68	10.497	2939	2941	2944	rBV2	392	283	0.03%	0.004%
69	10.606	2972	2975	2977	rBV	239	170	0.02%	0.002%
70	10.747	3017	3019	3022	rVB	383	222	0.03%	0.003%
71	10.770	3022	3026	3027	rBV	332	239	0.03%	0.003%
72	10.847	3046	3050	3052	rBV2	353	259	0.03%	0.004%
73	10.870	3055	3057	3062	rBV2	215	200	0.02%	0.003%
74	11.040	3106	3110	3116	rBV3	345	456	0.06%	0.007%
75	11.092	3123	3126	3130	rVB2	304	176	0.02%	0.003%
76	11.130	3133	3138	3139	rBV3	471	413	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033069.D
 Acq On : 24 Nov 2023 13:16
 Operator : SY/MD
 Sample : VIBLK258
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3181	rBV	537654	828097	100.00%	12.096%
78	11.400	3220	3222	3225	rVB3	530	231	0.03%	0.003%
79	11.561	3260	3272	3292	rBV	458506	724102	87.44%	10.577%
80	11.802	3345	3347	3350	rVB	462	181	0.02%	0.003%
81	11.841	3358	3359	3363	rVB2	345	214	0.03%	0.003%
82	11.892	3371	3375	3378	rBV2	266	258	0.03%	0.004%
83	11.908	3378	3380	3382	rBV	354	190	0.02%	0.003%
84	11.969	3398	3399	3402	rVB	486	228	0.03%	0.003%
85	12.030	3416	3418	3422	rVB	381	220	0.03%	0.003%
86	12.204	3462	3472	3477	rBV3	1585	2480	0.30%	0.036%
87	12.310	3503	3505	3507	rBV2	240	168	0.02%	0.002%
88	12.416	3535	3538	3542	rBV	429	268	0.03%	0.004%
89	12.564	3581	3584	3588	rVB2	502	335	0.04%	0.005%
90	12.583	3588	3590	3593	rBV	268	212	0.03%	0.003%
91	12.686	3618	3622	3626	rBV	459	439	0.05%	0.006%
92	12.866	3676	3678	3682	rBV3	458	209	0.03%	0.003%
93	13.217	3781	3787	3791	rBV3	762	949	0.11%	0.014%
94	13.358	3827	3831	3834	rBV2	580	502	0.06%	0.007%
95	13.442	3855	3857	3858	rBV2	574	229	0.03%	0.003%
96	13.683	3930	3932	3934	rBV3	636	388	0.05%	0.006%
97	13.760	3951	3956	3958	rBV	401	405	0.05%	0.006%
98	13.882	3990	3994	3995	rBV	476	310	0.04%	0.005%
99	14.413	4157	4159	4166	rVB6	813	618	0.07%	0.009%
100	14.487	4178	4182	4184	rBV2	513	380	0.05%	0.006%




Sum of corrected areas: 6845785

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033069.D
Acq On : 24 Nov 2023 13:16
Operator : SY/MD
Sample : VIBLK258
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

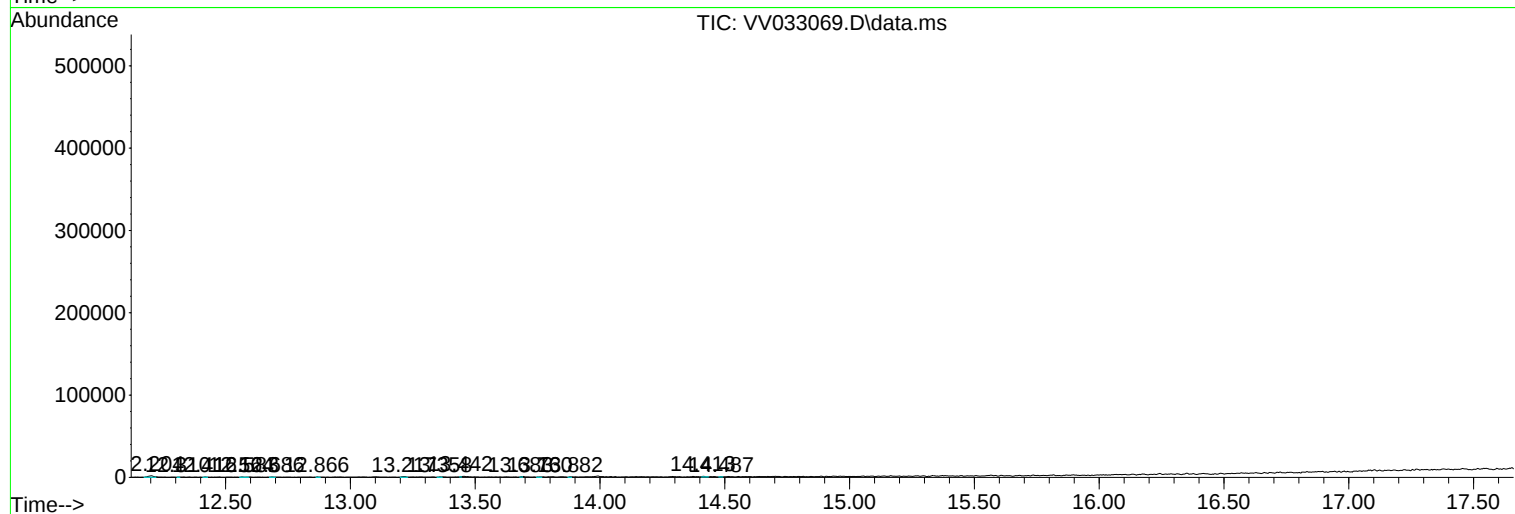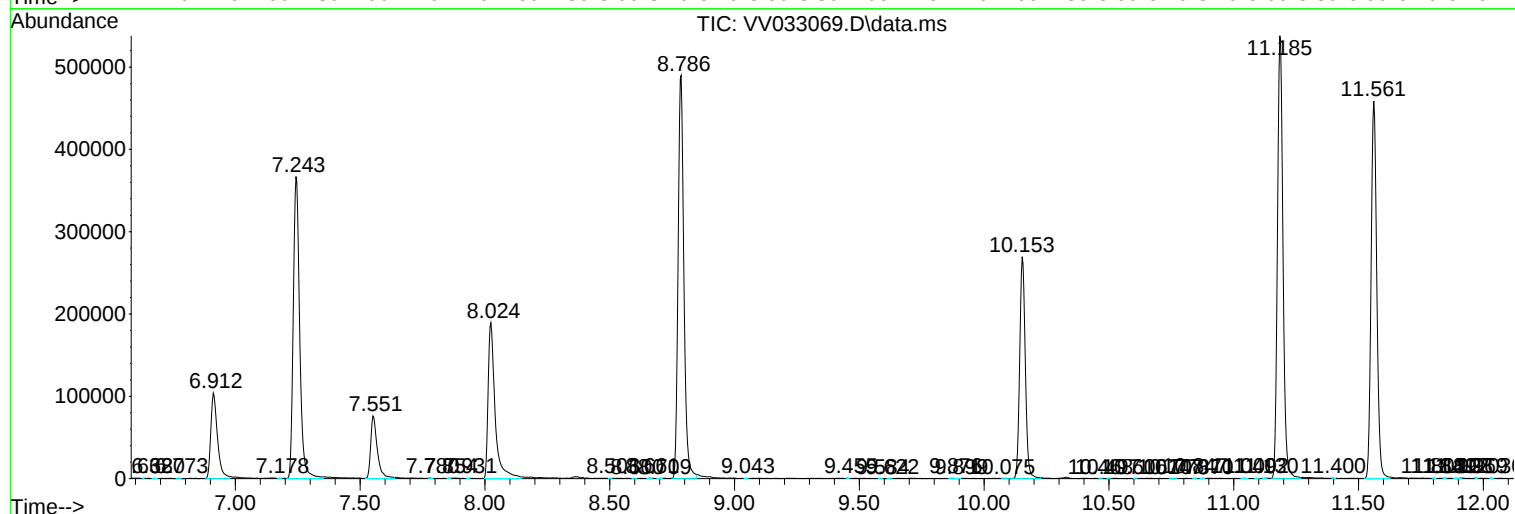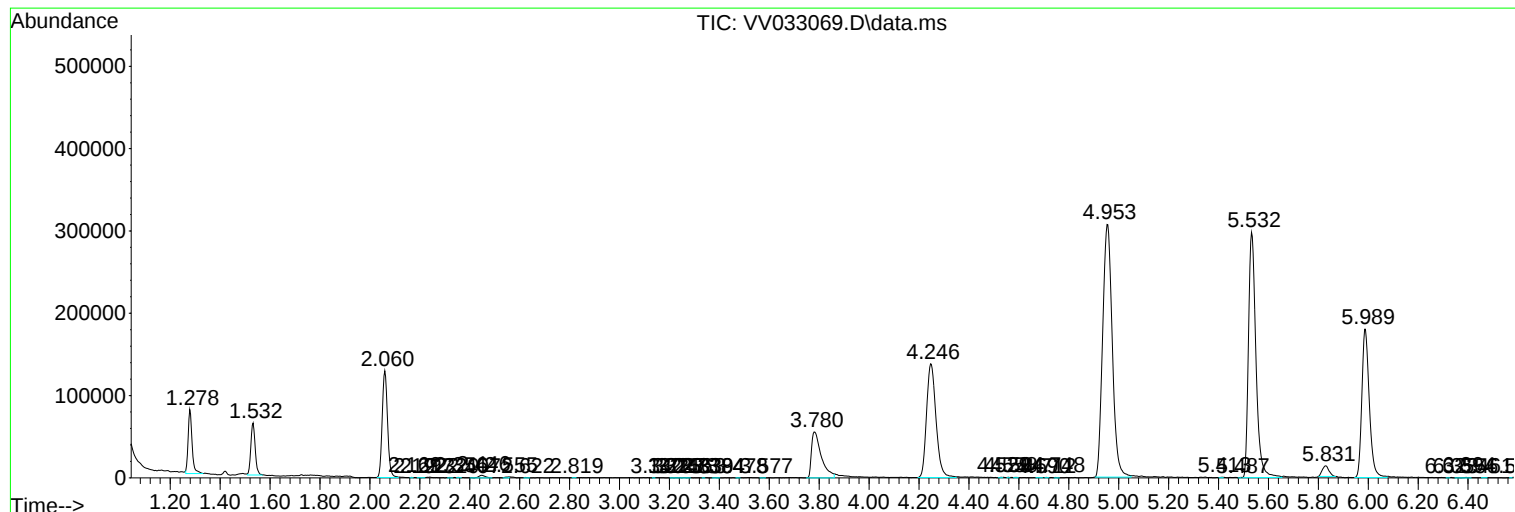

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033069.D
Acq On : 24 Nov 2023 13:16
Operator : SY/MD
Sample : VIBLK258
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
Data File : VV033069.D
Acq On : 24 Nov 2023 13:16
Operator : SY/MD
Sample : VIBLK258
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------