
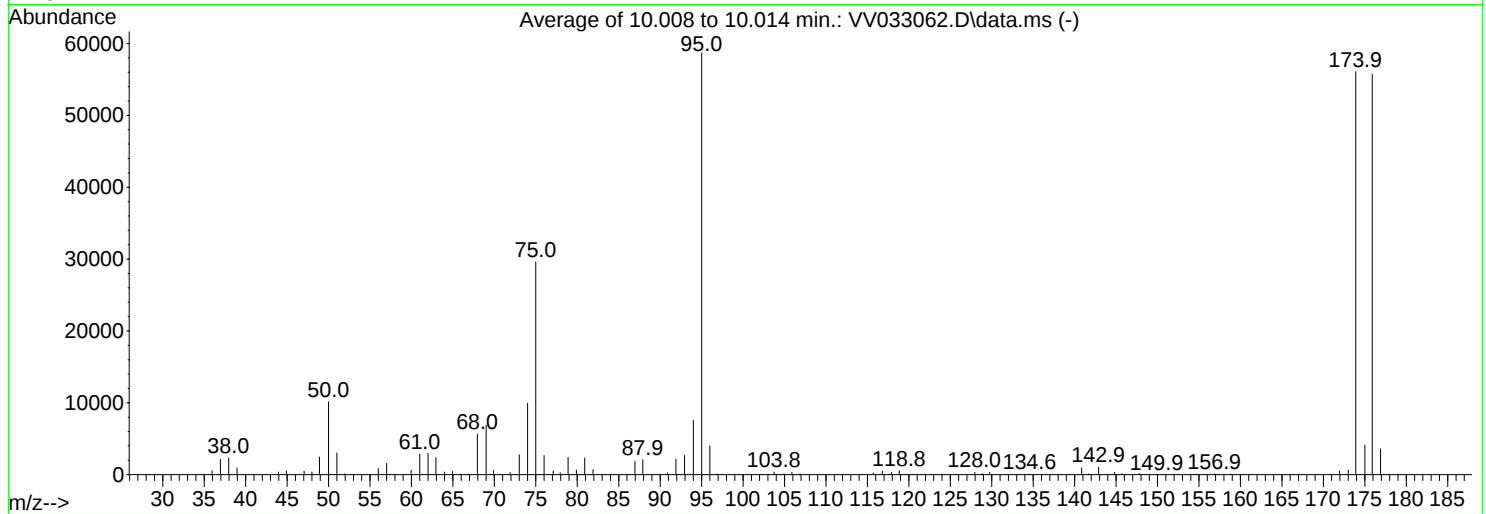


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112423\
 Data File : VV033062.D
 Acq On : 24 Nov 2023 09:14
 Operator : SY/MD
 Sample : BFB237
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB237

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis
 Last Update : Mon Nov 27 00:54:52 2023

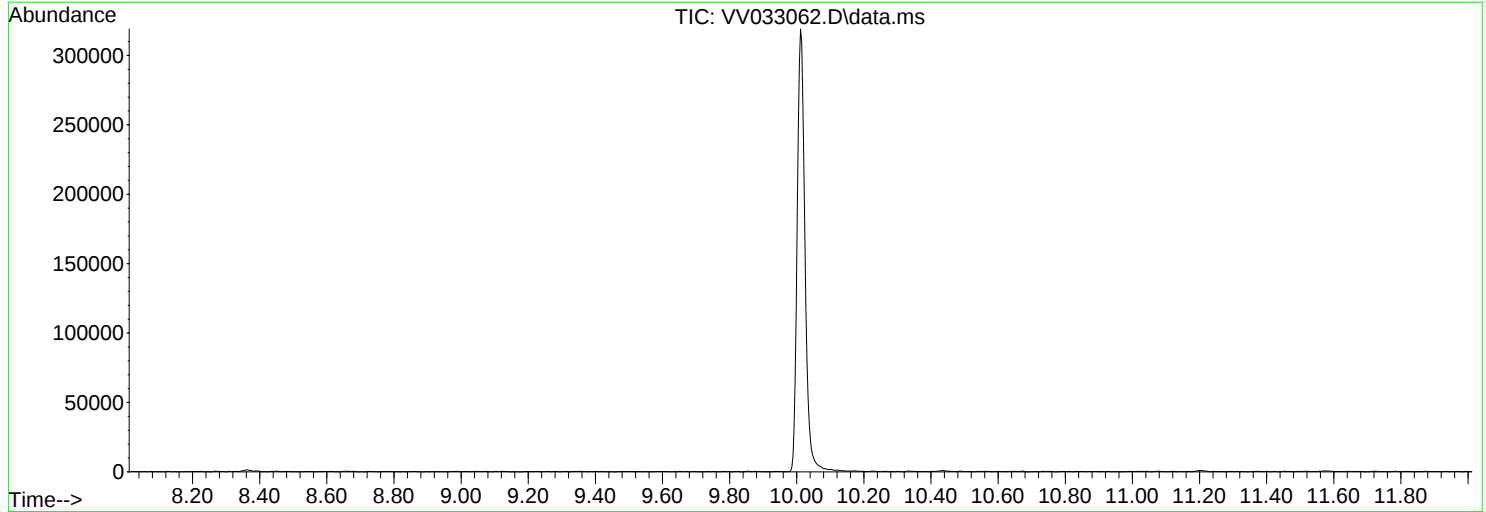

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	10149	PASS
75	95	30	80	50.4	29592	PASS
95	95	100	100	100.0	58704	PASS
96	95	5	9	6.8	4009	PASS
173	174	0.00	2	1.1	617	PASS
174	95	50	120	95.6	56112	PASS
175	174	5	9	7.3	4116	PASS
176	174	95	105	99.3	55733	PASS
177	176	5	10	6.4	3579	PASS

m/z	Abundance
43.80	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
35.90	559.0
36.90	2289.0
38.00	2217.0
39.00	865.0
44.00	503.0
44.90	478.0
47.00	444.0
48.00	303.0
48.90	2403.0
50.00	10068.0
51.00	2927.0
51.90	118.0
56.00	847.0
57.00	1562.0
60.00	673.0
61.00	2864.0
62.00	2807.0
63.00	2088.0
63.90	293.0
65.00	367.0
65.90	119.0
66.80	105.0
68.00	5656.0
69.00	6614.0
69.90	568.0
71.90	326.0
73.00	2650.0
74.00	9358.0
75.00	29160.0
76.00	2438.0
77.10	493.0
77.90	248.0
78.90	2183.0
79.90	686.0
80.90	2253.0
81.90	670.0
85.90	101.0
87.00	1751.0
87.90	2084.0
90.90	282.0
91.90	2107.0
93.00	2618.0
94.00	7335.0
95.00	57048.0
96.00	4180.0
103.80	314.0
104.90	130.0
105.80	286.0
106.80	107.0
115.00	114.0
115.70	241.0
116.80	493.0
117.90	322.0
118.80	581.0
127.90	283.0
128.80	139.0
129.70	270.0
134.90	114.0
140.80	859.0
142.90	916.0
144.80	254.0
145.70	168.0
147.80	130.0
156.90	109.0
172.00	529.0
173.90	53392.0
175.00	4117.0
175.90	52576.0
176.90	3390.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
35.90	579.0
37.00	2192.0
38.00	2396.0
39.00	964.0
44.00	544.0
44.90	541.0
47.10	489.0
48.00	405.0
48.90	2559.0
50.00	10494.0
51.00	3204.0
52.00	122.0
55.10	103.0
56.00	872.0
57.00	1613.0
59.90	668.0
61.00	2944.0
62.00	3076.0
63.00	2347.0
64.00	353.0
64.90	471.0
65.90	130.0
66.80	112.0
67.90	5775.0
69.00	7217.0
69.90	588.0
71.90	296.0
73.00	2838.0
74.00	10301.0
75.00	30552.0
76.00	2779.0
77.10	520.0
77.90	307.0
78.90	2514.0
79.90	654.0
80.90	2412.0
81.90	723.0
85.90	114.0
86.90	1930.0
87.90	2194.0
90.90	244.0
91.90	2225.0
93.00	2727.0
94.00	7747.0
95.00	60752.0
96.00	4146.0
96.80	105.0
103.00	114.0
103.70	394.0
105.00	159.0
105.90	347.0
106.90	135.0
115.00	112.0
115.70	254.0
116.80	534.0
117.90	341.0
118.80	573.0
127.90	335.0
128.90	127.0
129.80	319.0
134.60	144.0
140.80	1006.0
141.70	149.0
142.90	1088.0
144.80	331.0
145.70	157.0
147.80	149.0
151.80	105.0
154.70	104.0
156.90	138.0
158.80	101.0
171.00	101.0
171.90	517.0
173.00	920.0
173.90	57976.0
175.00	4160.0
175.90	57520.0
176.90	3708.0
177.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
36.00	514.0
37.00	1985.0
37.90	2358.0
38.90	985.0
44.00	493.0
44.90	504.0
45.90	111.0
47.10	508.0
48.00	447.0
48.90	2374.0
50.00	9885.0
51.00	2961.0
52.00	114.0
55.00	118.0
56.00	896.0
57.00	1518.0
58.00	105.0
59.90	631.0
61.00	2803.0
62.00	2986.0
62.90	2634.0
64.10	404.0
64.90	524.0
67.90	5510.0
69.00	6790.0
69.90	505.0
71.90	272.0
73.00	2794.0
74.00	10151.0
75.00	29064.0
76.00	2723.0
77.10	505.0
78.00	278.0
78.90	2520.0
79.90	600.0
80.90	2281.0
81.90	724.0
86.90	1896.0
87.90	2031.0
90.90	220.0
91.90	2124.0
92.90	2664.0
94.00	7620.0
95.00	58312.0
96.00	3702.0
96.80	154.0
103.70	393.0
105.00	140.0
106.00	366.0
106.90	119.0
115.70	245.0
116.80	541.0
117.90	289.0
118.90	534.0
128.00	360.0
128.90	129.0
129.80	327.0
134.60	160.0
140.90	1036.0
141.70	168.0
142.90	1044.0
144.80	353.0
145.70	118.0
147.80	181.0
149.90	118.0
154.70	122.0
156.90	155.0
158.80	101.0
171.00	115.0
171.90	485.0
173.00	932.0
173.90	56968.0
175.00	4071.0
175.90	57104.0
176.90	3640.0
177.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237