

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
 Data File : VV038323.D
 Acq On : 24 Nov 2024 11:36
 Operator : SY/MD
 Sample : VV1124WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	83	rBV	111004	119005	15.10%	1.806%
2	1.532	145	153	164	rBV	103230	121412	15.40%	1.842%
3	2.053	306	315	333	rVB	188907	281035	35.66%	4.265%
4	3.802	849	859	890	rBV	75666	257685	32.69%	3.910%
5	4.239	978	995	1028	rBV	137673	366664	46.52%	5.564%
6	4.950	1199	1216	1264	rBV3	295898	788169	100.00%	11.960%
7	5.529	1382	1396	1431	rBV	246371	560981	71.18%	8.513%
8	5.982	1521	1537	1556	rBV	174215	380691	48.30%	5.777%
9	6.915	1812	1827	1858	rBV2	65755	156028	19.80%	2.368%
10	7.236	1917	1927	1958	rBV	299343	575706	73.04%	8.736%
11	7.558	2018	2027	2050	rBV	37348	83761	10.63%	1.271%
12	8.024	2163	2172	2222	rBV	263120	666749	84.59%	10.118%
13	8.779	2396	2407	2449	rBV	413749	753331	95.58%	11.432%
14	10.146	2817	2832	2856	rBV	144565	248231	31.49%	3.767%
15	11.178	3144	3153	3180	rBV	365751	624178	79.19%	9.472%
16	11.554	3258	3270	3293	rBV	317260	545679	69.23%	8.280%
17	13.207	3776	3784	3792	rBV5	8201	13893	1.76%	0.211%
18	13.448	3848	3859	3876	rBV3	13204	30540	3.87%	0.463%
19	13.686	3922	3933	3943	rBV5	8504	16213	2.06%	0.246%




Sum of corrected areas: 6589951

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038323.D
Acq On : 24 Nov 2024 11:36
Operator : SY/MD
Sample : VV1124WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

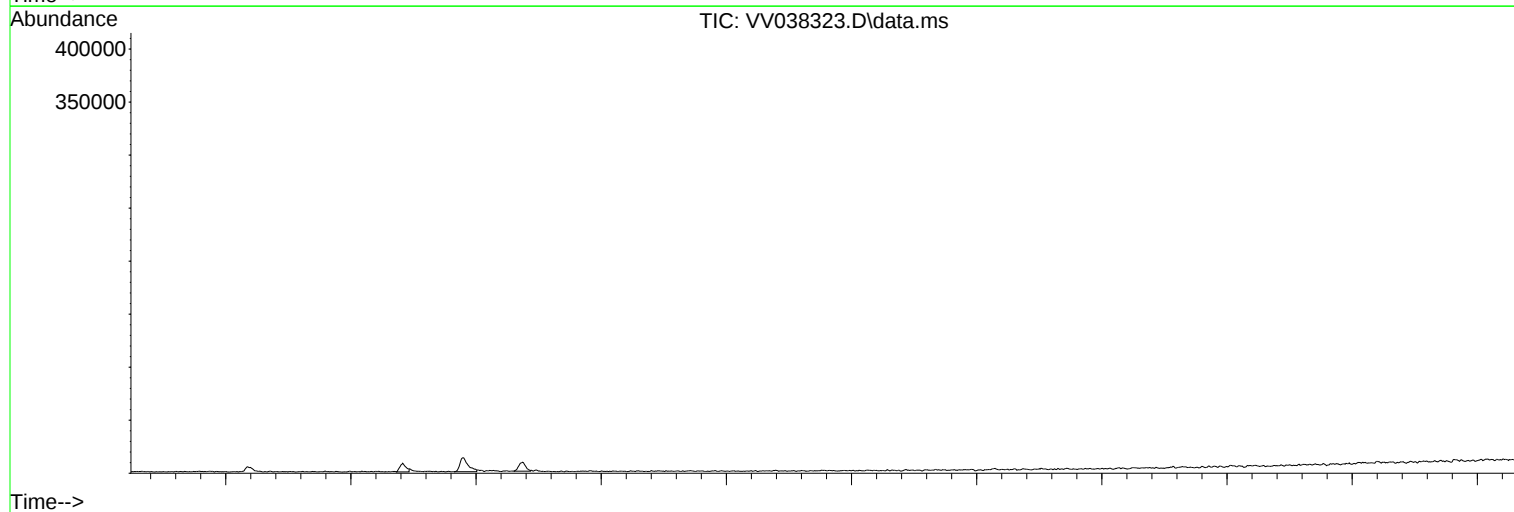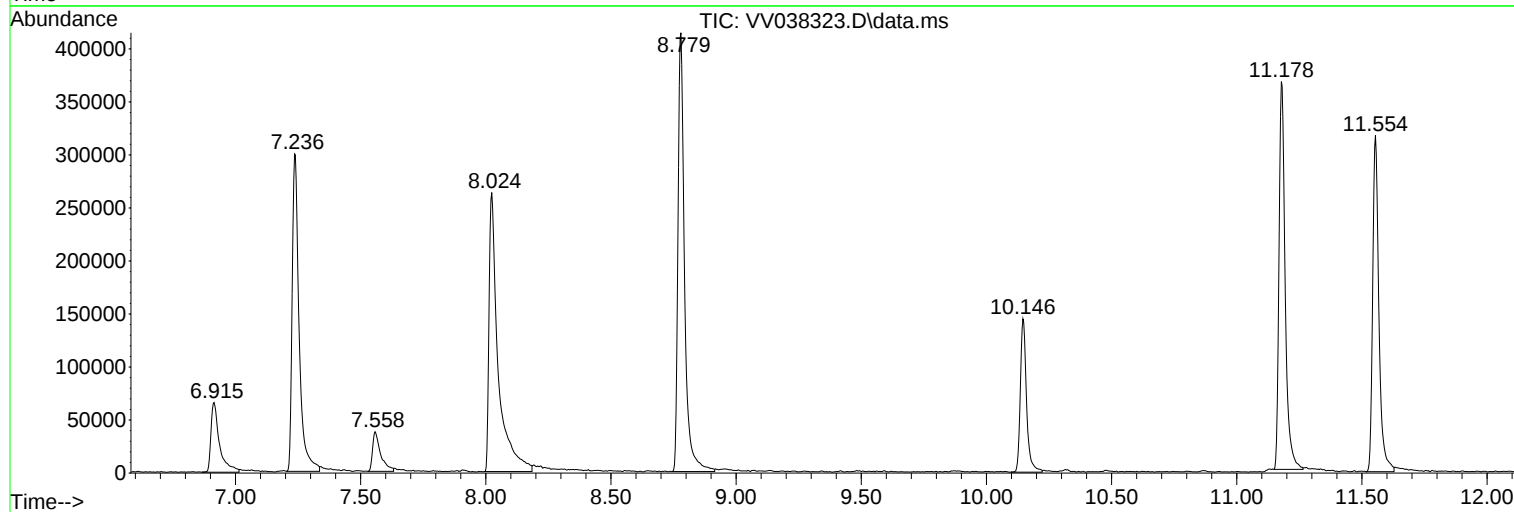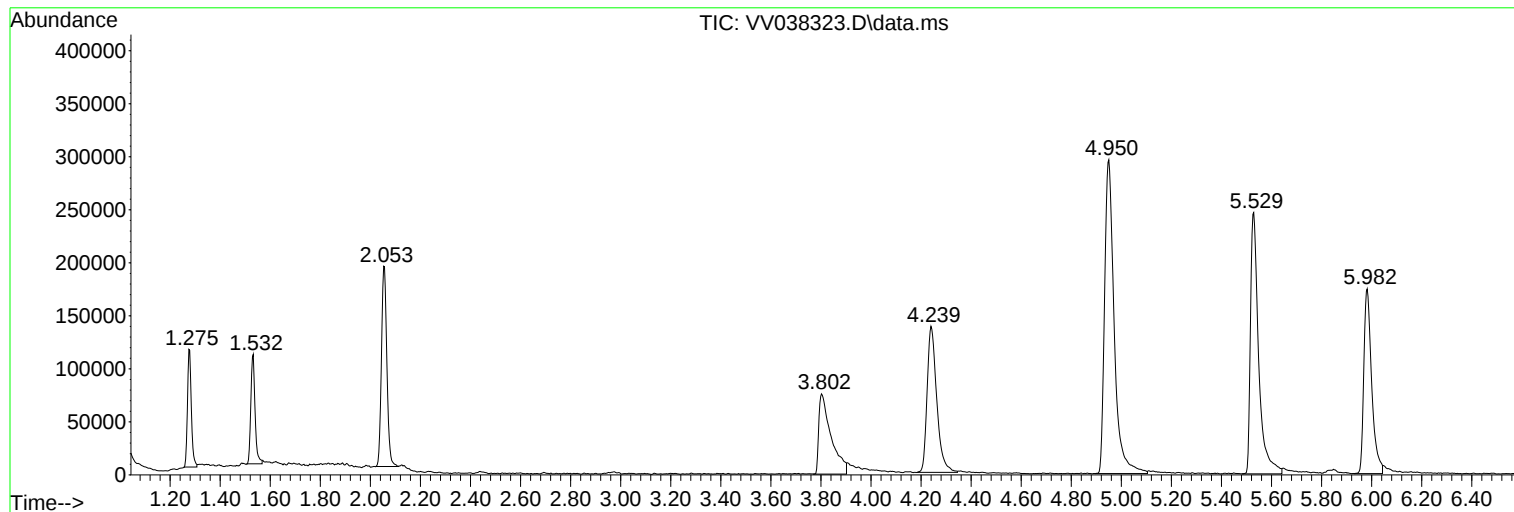

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038323.D
Acq On : 24 Nov 2024 11:36
Operator : SY/MD
Sample : VV1124WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038323.D
Acq On : 24 Nov 2024 11:36
Operator : SY/MD
Sample : VV1124WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
