

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
 Data File : VV038324.D
 Acq On : 24 Nov 2024 12:04
 Operator : SY/MD
 Sample : P4884-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3M6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.712	199	209	227	rBV	1725103	2306628	15.57%	9.246%
2	1.854	238	253	305	rBV	6277060	14816138	100.00%	59.387%
3	2.056	308	316	331	rVB2	232390	381629	2.58%	1.530%
4	2.696	501	515	536	rBV	96277	203344	1.37%	0.815%
5	3.105	626	642	667	rBV2	111067	239070	1.61%	0.958%
6	3.786	843	854	893	rBV	92307	306602	2.07%	1.229%
7	4.243	981	996	1027	rBV2	144116	403857	2.73%	1.619%
8	4.503	1061	1077	1096	rBV4	85769	229036	1.55%	0.918%
9	4.950	1202	1216	1243	rBV2	303063	786921	5.31%	3.154%
10	5.529	1385	1396	1432	rBV	241073	546636	3.69%	2.191%
11	5.831	1479	1490	1515	rBV2	106279	246972	1.67%	0.990%
12	5.982	1524	1537	1563	rBV	182409	392774	2.65%	1.574%
13	6.911	1816	1826	1846	rBV	68765	151195	1.02%	0.606%
14	7.236	1916	1927	1946	rBV	306236	583051	3.94%	2.337%
15	7.899	2116	2133	2156	rBV2	265764	476101	3.21%	1.908%
16	8.018	2162	2170	2211	rBV	281695	637770	4.30%	2.556%
17	8.780	2393	2407	2436	rBV	415484	782069	5.28%	3.135%
18	10.146	2822	2832	2850	rBV	147981	250530	1.69%	1.004%
19	11.178	3142	3153	3180	rBV	365078	630462	4.26%	2.527%
20	11.554	3258	3270	3291	rBV	332554	577730	3.90%	2.316%

Sum of corrected areas: 24948515




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038324.D
Acq On : 24 Nov 2024 12:04
Operator : SY/MD
Sample : P4884-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

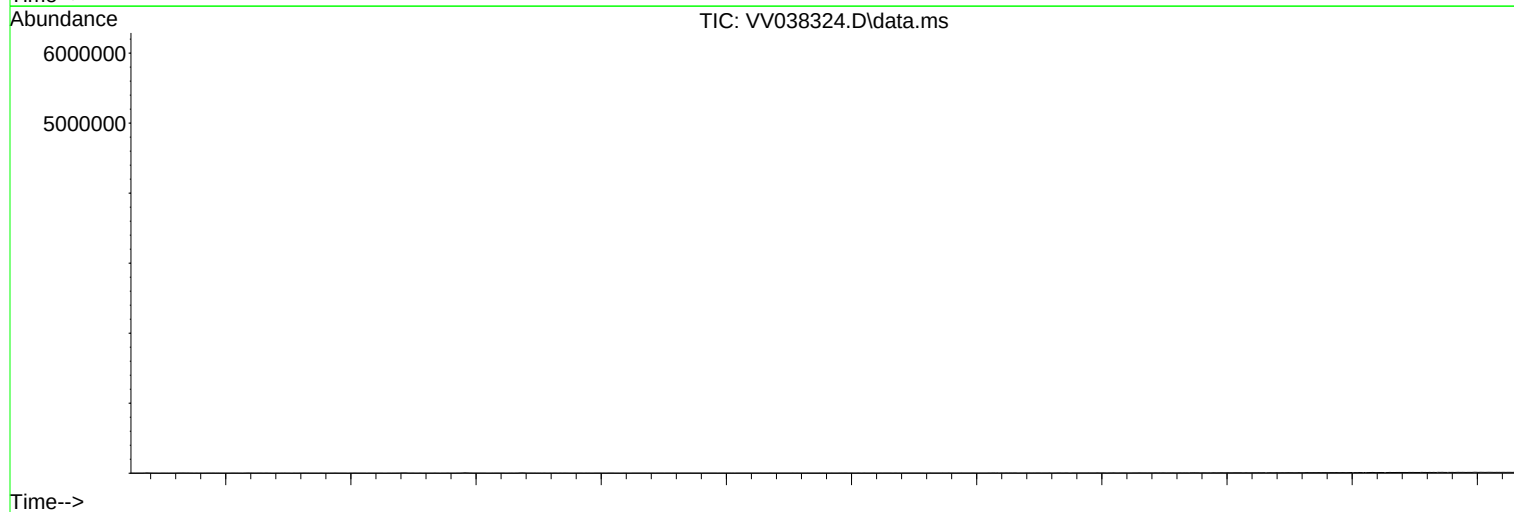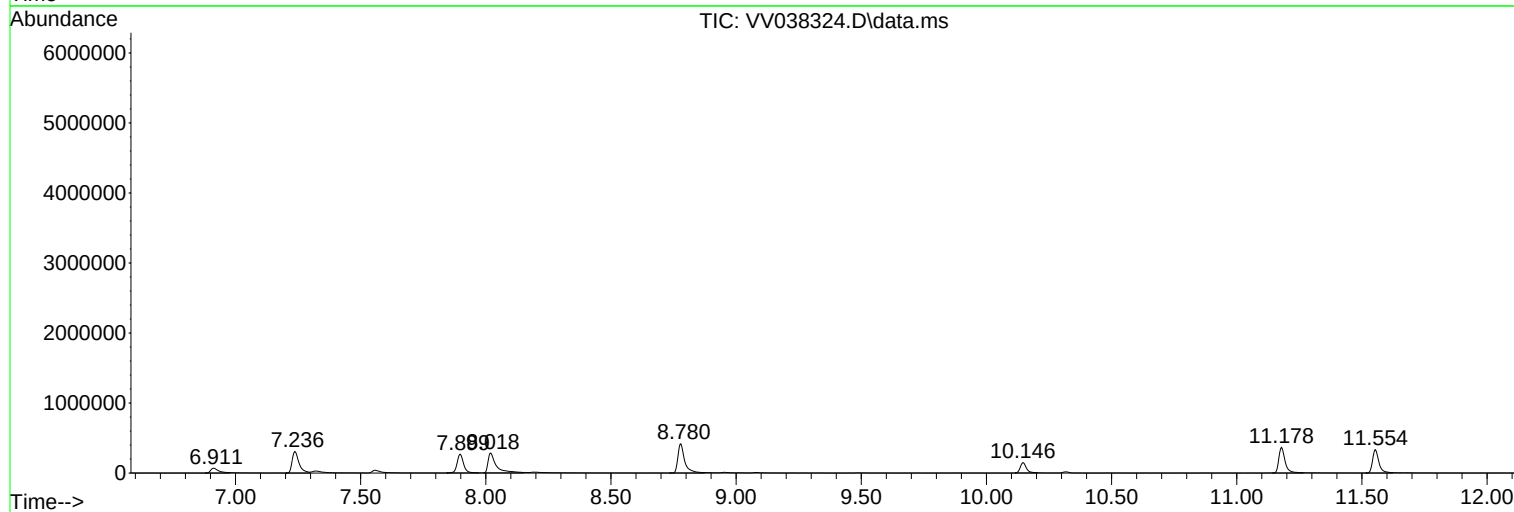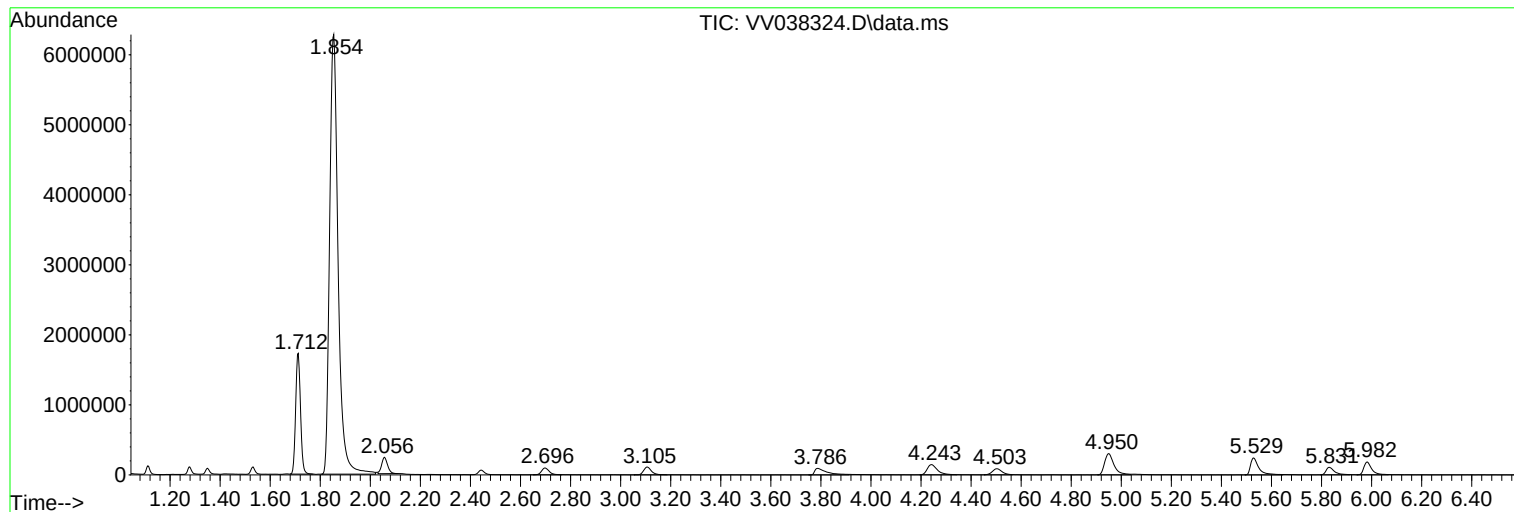

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038324.D
Acq On : 24 Nov 2024 12:04
Operator : SY/MD
Sample : P4884-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038324.D
Acq On : 24 Nov 2024 12:04
Operator : SY/MD
Sample : P4884-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc