

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
 Data File : VV038325.D
 Acq On : 24 Nov 2024 12:28
 Operator : SY/MD
 Sample : P4884-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3M5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	85	rBV	106677	117613	2.56%	0.666%
2	1.529	144	152	161	rBV	99498	116463	2.53%	0.659%
3	1.709	198	208	235	rVB	3490772	4603245	100.00%	26.056%
4	1.989	254	295	296	rBV2	282710	1168961	25.39%	6.617%
5	2.056	310	316	370	rVB2	490084	1366197	29.68%	7.733%
6	2.439	424	435	459	rBV	278334	466908	10.14%	2.643%
7	2.696	498	515	541	rBV	278667	593442	12.89%	3.359%
8	3.104	628	642	666	rBV	196073	421817	9.16%	2.388%
9	3.805	850	860	903	rBV4	114786	396096	8.60%	2.242%
10	4.243	975	996	1027	rBV2	138814	395658	8.60%	2.240%
11	4.503	1060	1077	1105	rBV2	120171	318126	6.91%	1.801%
12	4.950	1201	1216	1239	rBV3	287772	752681	16.35%	4.260%
13	5.529	1386	1396	1427	rBV	244440	545793	11.86%	3.089%
14	5.828	1478	1489	1523	rBV2	224992	500463	10.87%	2.833%
15	5.982	1523	1537	1567	rVV2	171396	373529	8.11%	2.114%
16	6.911	1817	1826	1855	rBV	64480	145400	3.16%	0.823%
17	7.239	1916	1928	1944	rBV	298047	562194	12.21%	3.182%
18	7.317	1944	1952	1983	rVB	81607	177247	3.85%	1.003%
19	7.558	2019	2027	2044	rBV	38115	80370	1.75%	0.455%
20	7.895	2112	2132	2158	rBV	687592	1202590	26.12%	6.807%
21	8.024	2163	2172	2216	rVV	278837	649204	14.10%	3.675%
22	8.779	2396	2407	2447	rBV2	427817	897274	19.49%	5.079%
23	8.947	2451	2459	2475	rVB	27298	50481	1.10%	0.286%
24	9.072	2487	2498	2521	rBV2	47132	91505	1.99%	0.518%
25	10.146	2815	2832	2856	rBV	146454	265021	5.76%	1.500%
26	11.178	3144	3153	3180	rBV	381222	653722	14.20%	3.700%
27	11.487	3240	3249	3260	rBV3	41639	91695	1.99%	0.519%
28	11.554	3260	3270	3304	rVB	347872	662872	14.40%	3.752%




Sum of corrected areas: 17666567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038325.D
Acq On : 24 Nov 2024 12:28
Operator : SY/MD
Sample : P4884-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

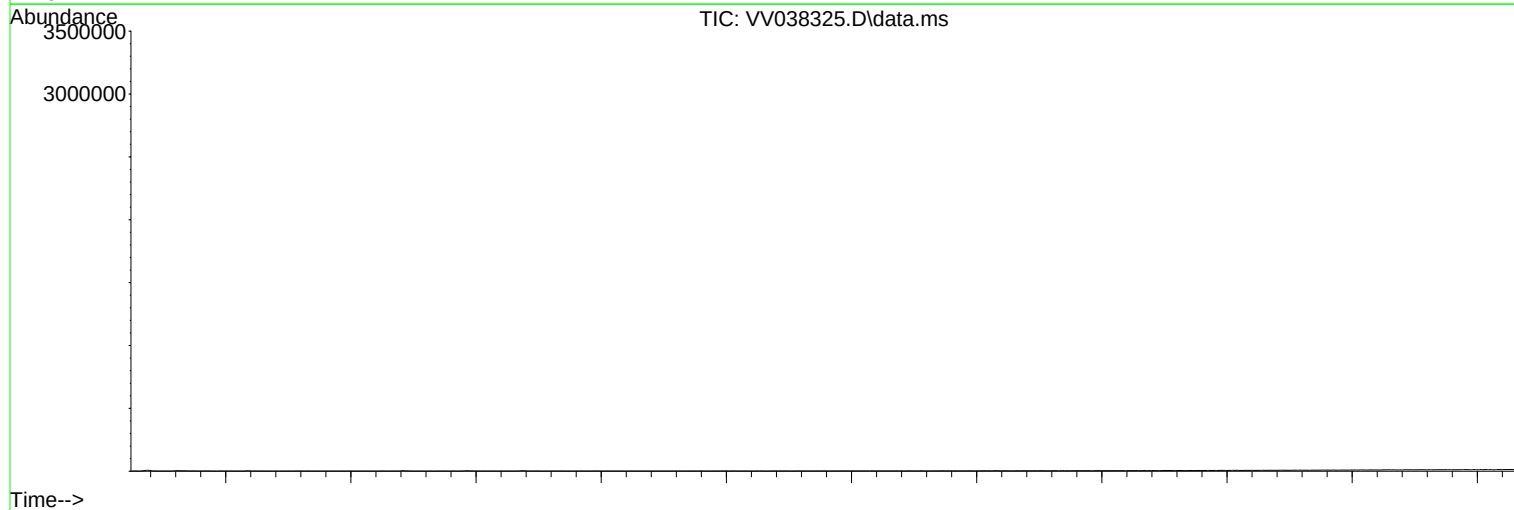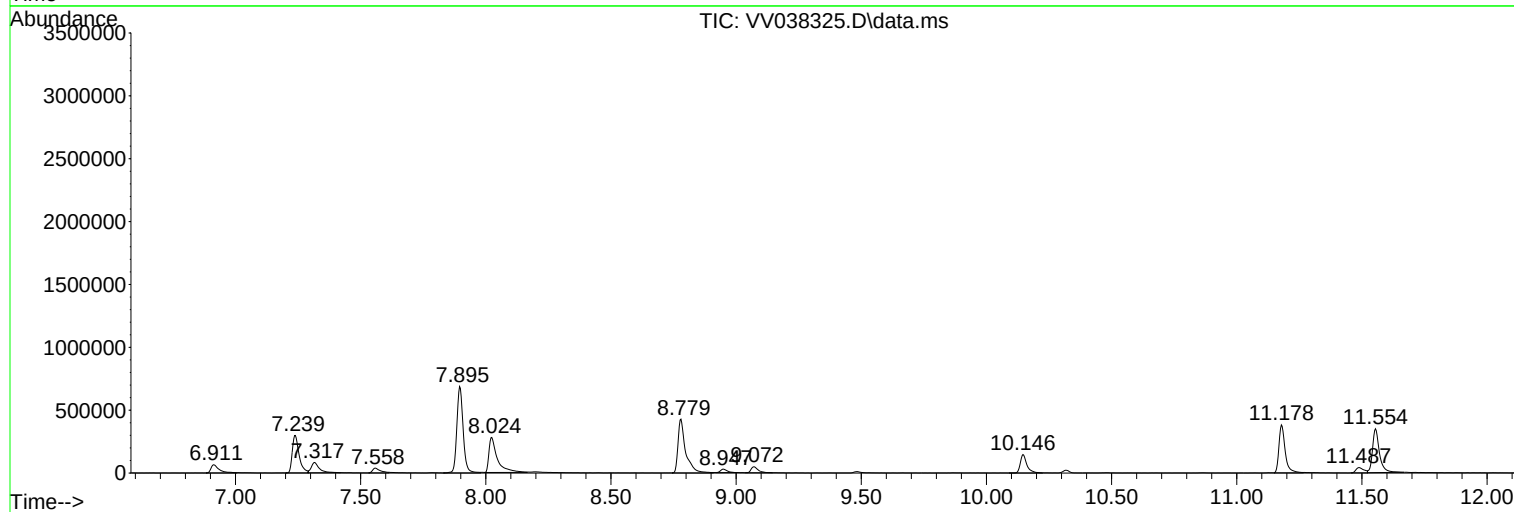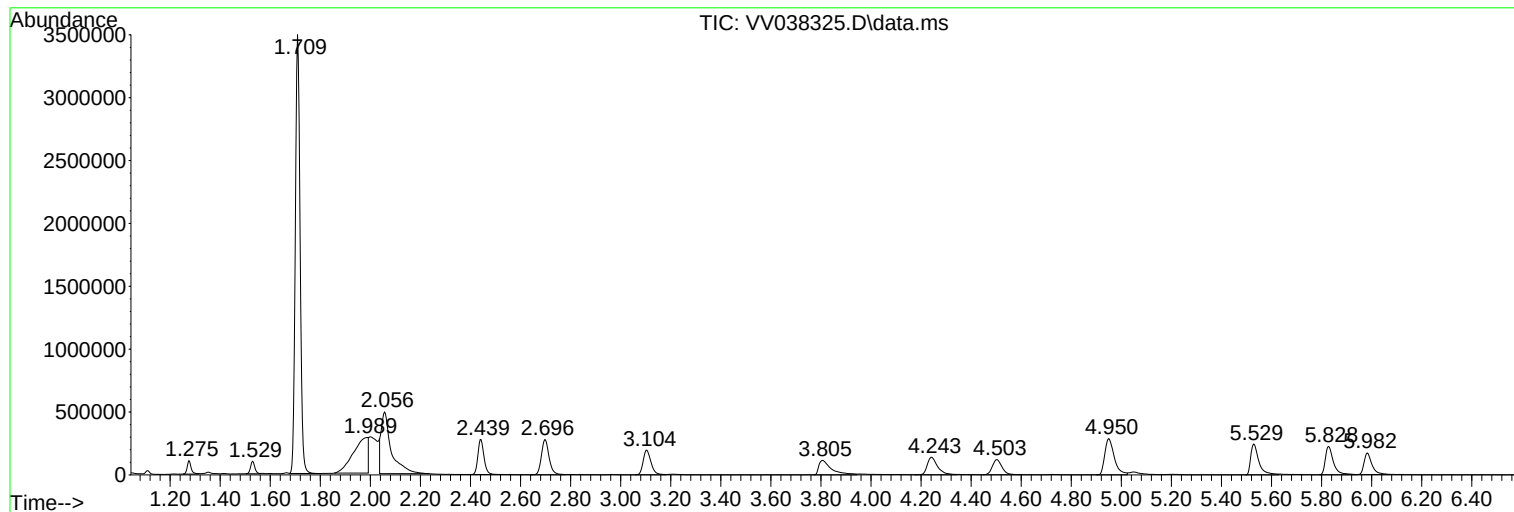

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038325.D
Acq On : 24 Nov 2024 12:28
Operator : SY/MD
Sample : P4884-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038325.D
Acq On : 24 Nov 2024 12:28
Operator : SY/MD
Sample : P4884-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc