

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
 Data File : VV038326.D
 Acq On : 24 Nov 2024 12:50
 Operator : SY/MD
 Sample : VIBLK202
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK202

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	85	rBV	109158	114998	15.24%	1.765%
2	1.529	145	152	163	rVB	93695	110840	14.69%	1.701%
3	1.709	202	208	215	rBV4	5702	8183	1.08%	0.126%
4	1.867	249	257	261	rBV3	6658	11596	1.54%	0.178%
5	2.053	303	315	329	rBV	183285	271478	35.98%	4.167%
6	3.789	843	855	894	rBV	89653	297132	39.38%	4.560%
7	4.243	980	996	1028	rBV	134730	366373	48.56%	5.623%
8	4.950	1201	1216	1243	rBV2	286611	754513	100.00%	11.580%
9	5.529	1385	1396	1422	rBV	241572	527583	69.92%	8.097%
10	5.982	1521	1537	1569	rBV	169849	380550	50.44%	5.841%
11	6.915	1816	1827	1852	rBV2	64006	143560	19.03%	2.203%
12	7.239	1917	1928	1958	rBV	286638	553517	73.36%	8.496%
13	7.558	2019	2027	2048	rBV3	37736	85816	11.37%	1.317%
14	7.870	2110	2124	2130	rBV3	6325	12077	1.60%	0.185%
15	8.021	2163	2171	2216	rBV	304606	695275	92.15%	10.671%
16	8.780	2397	2407	2439	rBV	412364	732507	97.08%	11.243%
17	10.146	2821	2832	2859	rBV	152361	254227	33.69%	3.902%
18	10.317	2876	2885	2898	rVB2	13920	20944	2.78%	0.321%
19	11.178	3143	3153	3185	rBV	372224	627377	83.15%	9.629%
20	11.554	3260	3270	3296	rVB	323249	546846	72.48%	8.393%




Sum of corrected areas: 6515392

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038326.D
Acq On : 24 Nov 2024 12:50
Operator : SY/MD
Sample : VIBLK202
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

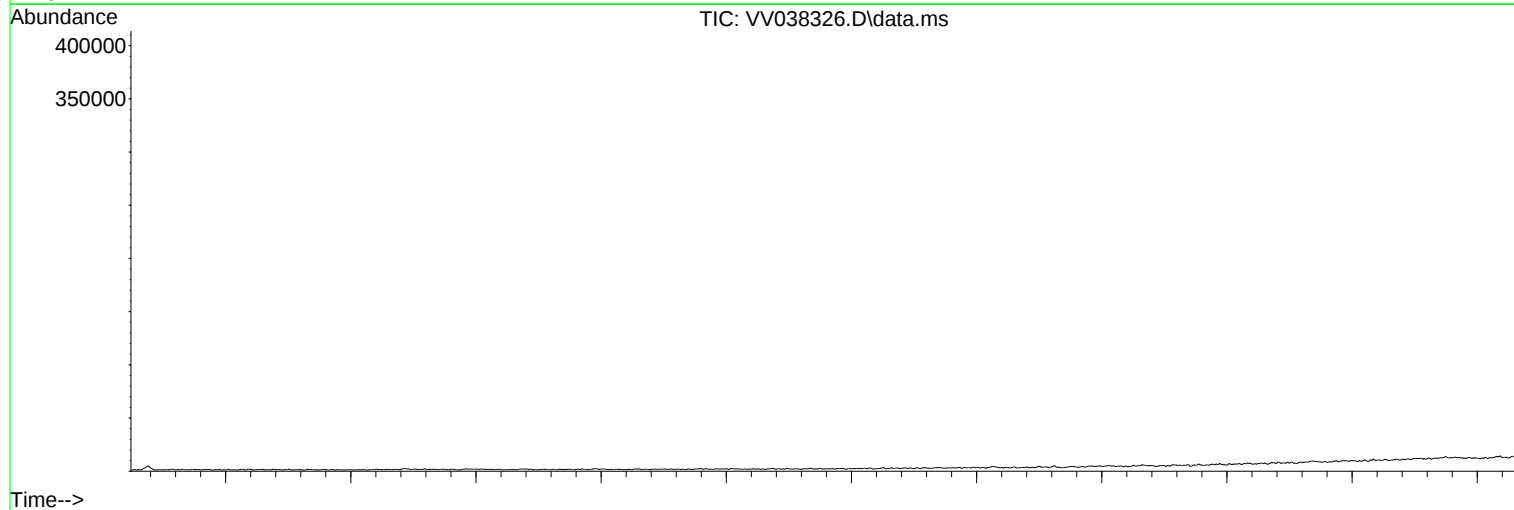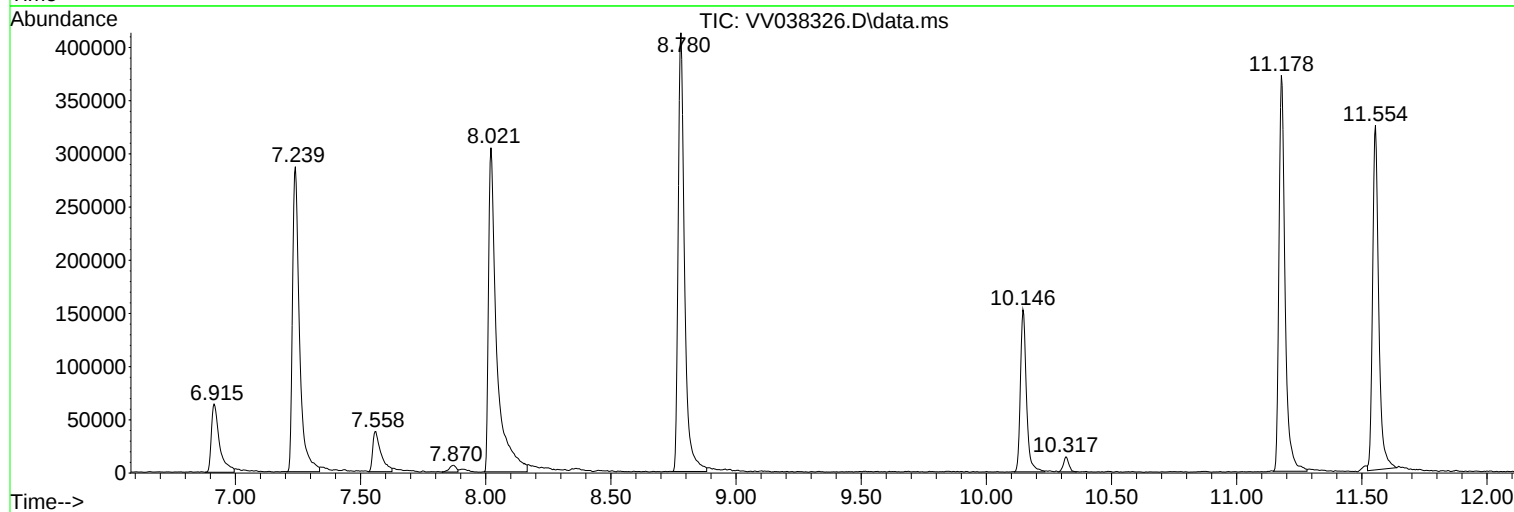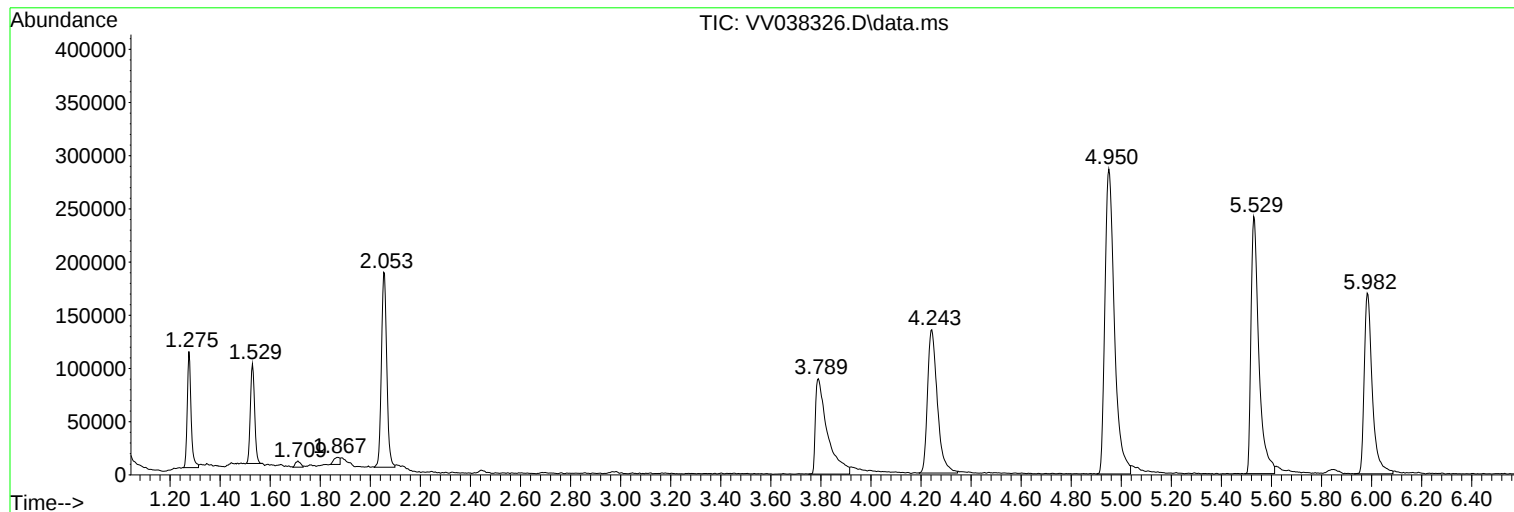

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038326.D
Acq On : 24 Nov 2024 12:50
Operator : SY/MD
Sample : VIBLK202
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112424\
Data File : VV038326.D
Acq On : 24 Nov 2024 12:50
Operator : SY/MD
Sample : VIBLK202
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc