

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112519\
 Data File : VV013757.D
 Acq On : 25 Nov 2019 11:37
 Operator : SY/MD
 Sample : VV1125WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK31

Quant Time: Nov 26 04:51:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 26 04:36:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	386938	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	375167	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	173569	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	106783	4.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.20%
7) Chloroethane-d5	1.58	69	99110	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.13	63	144258	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.60%
20) 2-Butanone-d5	3.96	46	225950	45.38	ug/L	0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.76%
24) Chloroform-d	4.40	84	220503	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	5.08	65	110849	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
32) Benzene-d6	5.09	84	439527	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
36) 1,2-Dichloropropane-d6	6.11	67	135938	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.35	98	372027	4.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.00%
43) trans-1,3-Dichloropropene-	7.66	79	47222	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
46) 2-Hexanone-d5	8.13	63	183391	44.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.56%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	93738	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	158564	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	7981	0.313 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112519\
Data File : VV013757.D
Acq On : 25 Nov 2019 11:37
Operator : SY/MD
Sample : VV1125WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK31

Quant Time: Nov 26 04:51:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 26 04:36:55 2019
Response via : Initial Calibration

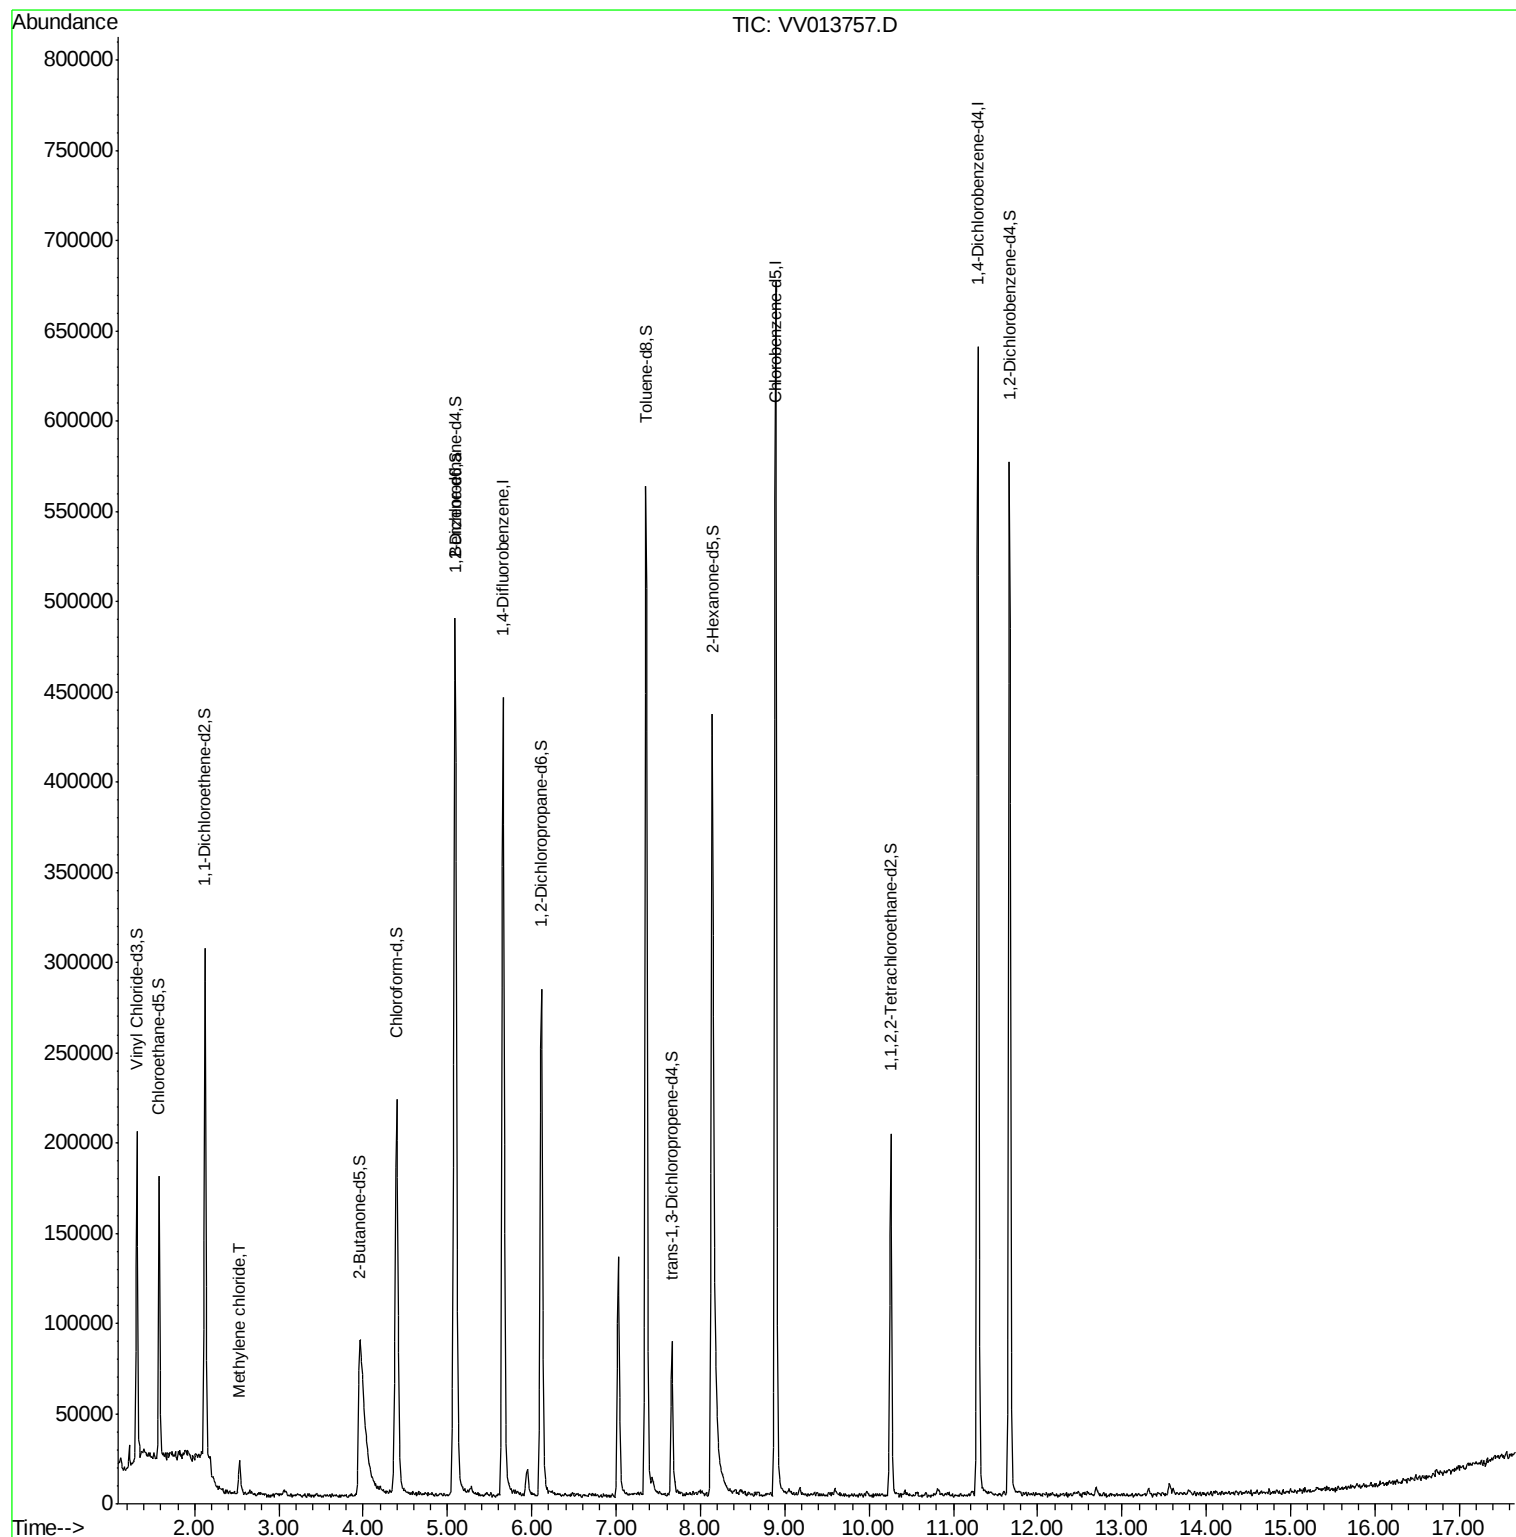

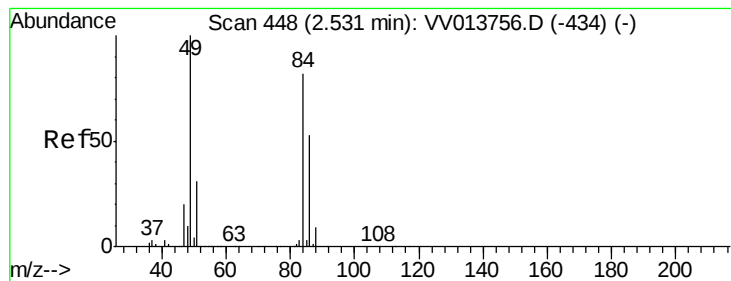

#16

Methylene chloride

Concen: 0.313 ug/L

RT: 2.53 min Scan# 448

Delta R.T. -0.00 min

Lab File: VV013757.D

Acq: 25 Nov 2019 11:37

Instrument :

MSVOA_V

ClientSampleId :

VBLK31

Tot Ion: 84 Resp: 7981

Ion Ratio Lower Upper

84 100

86 66.5 44.0 81.6

49 112.4 81.5 151.5

