


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112519\
Data File : VV013755.D
Acq On : 25 Nov 2019 08:59
Operator : SY/MD
Sample : BFB38
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB38

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Nov 26 14:16:20 2019

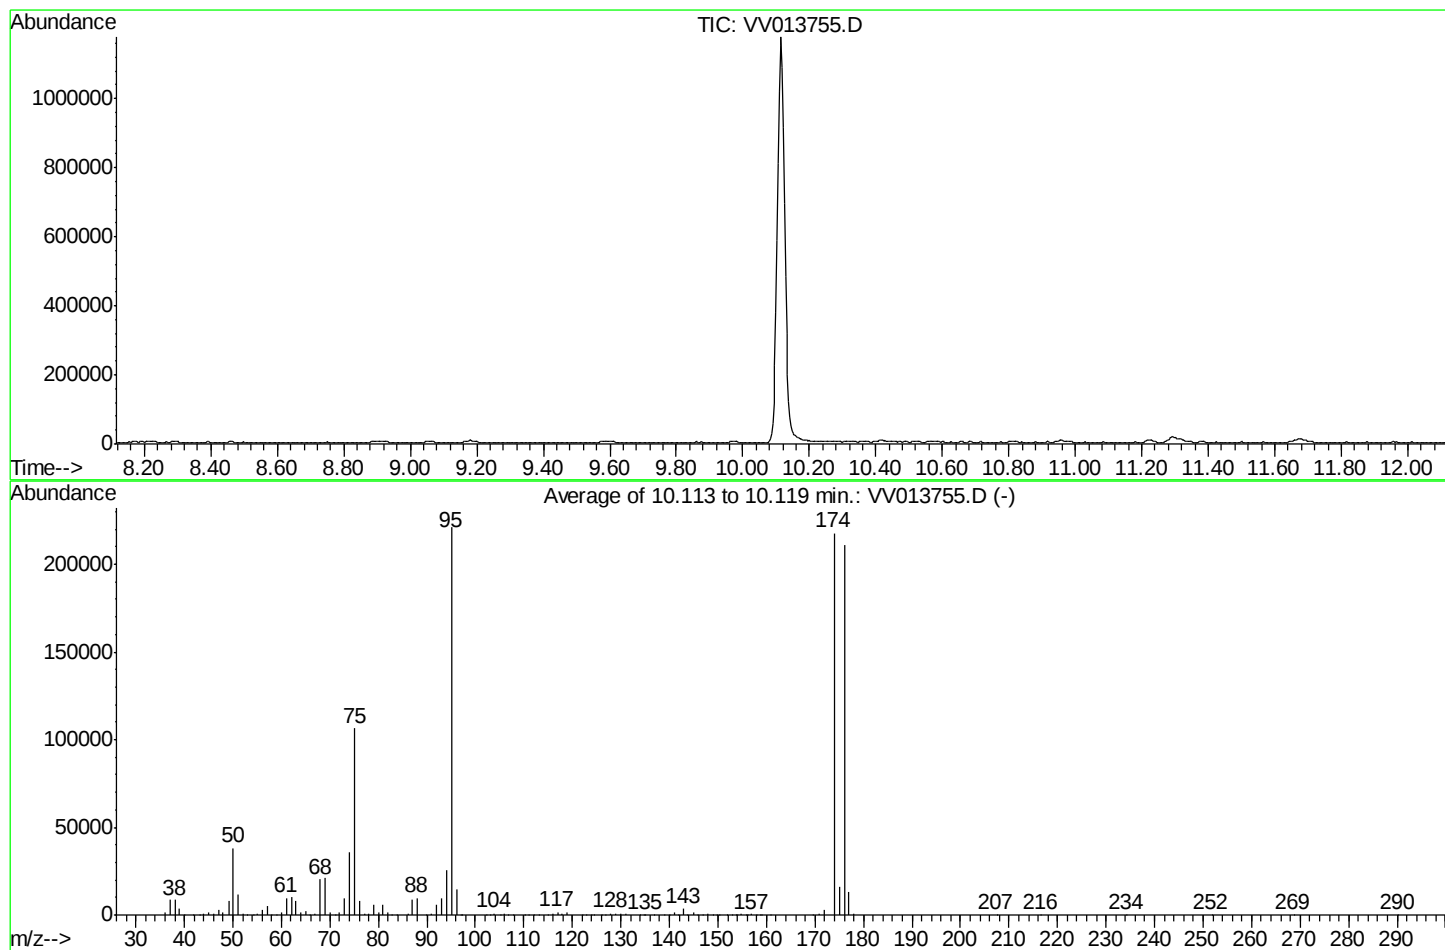

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	38144	PASS
75	95	30	80	48.2	106504	PASS
95	95	100	100	100.0	221098	PASS
96	95	5	9	6.5	14280	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.5	217856	PASS
175	174	5	9	7.5	16393	PASS
176	174	95	101	96.8	210837	PASS
177	176	5	9	6.4	13498	PASS

m/z	Abundance
36.00	1727.0
37.10	8655.0
38.10	9148.0
39.00	3612.0
40.00	904.0
42.10	152.0
43.20	154.0
44.00	1787.0
45.00	1505.0
46.20	404.0
47.00	2984.0
48.00	1696.0
49.10	8411.0
50.10	39560.0
51.00	12194.0
52.00	737.0
53.00	337.0
55.10	628.0
56.00	2984.0
57.10	5312.0
58.00	360.0
58.90	131.0
60.10	1835.0
61.00	9931.0
62.10	10323.0
63.10	8818.0
64.00	1576.0
65.00	2155.0
65.90	170.0
67.00	746.0
68.00	21264.0
69.10	21728.0
70.00	1444.0
71.20	126.0
72.10	1270.0
73.10	9652.0
74.00	36896.0
75.10	108152.0
76.10	8598.0
77.00	1293.0
77.90	1171.0
79.00	6075.0
80.00	1587.0
81.00	6345.0
82.00	1320.0
82.80	191.0
83.90	147.0
86.10	610.0
87.00	8962.0
88.00	10551.0
89.90	168.0
91.00	799.0
92.10	5692.0
93.00	9356.0
94.00	26112.0
95.00	224768.0
96.10	14532.0
97.00	406.0
102.30	106.0
103.00	132.0
104.00	1003.0
105.00	421.0
105.90	897.0
106.80	150.0
107.90	112.0
110.00	184.0
110.80	216.0
112.20	140.0
113.00	176.0
115.00	294.0
116.00	722.0
117.00	1632.0
117.90	769.0
118.90	1683.0
122.80	131.0
123.80	243.0
124.30	158.0
126.10	107.0
126.70	110.0
127.80	854.0
128.90	426.0
130.00	667.0
130.90	414.0
134.00	140.0
134.80	408.0
136.90	417.0
138.80	141.0
140.10	291.0
141.00	1754.0
141.90	258.0
142.90	3479.0
144.90	1478.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

145.80	494.0
146.90	347.0
147.90	715.0
148.80	207.0
149.70	198.0
150.20	215.0
151.90	184.0
152.90	200.0
153.80	148.0
154.80	596.0
156.20	179.0
156.90	577.0
157.90	109.0
158.80	229.0
159.10	260.0
160.90	272.0
169.60	177.0
171.00	609.0
172.00	3220.0
174.00	215040.0
175.00	16448.0
176.00	209088.0
177.00	13588.0
177.90	485.0
234.20	110.0
290.20	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
35.30	148.0
36.00	1931.0
37.10	8678.0
38.10	8821.0
39.00	3514.0
40.10	817.0
40.70	158.0
42.00	181.0
43.00	179.0
44.00	1781.0
45.00	1702.0
46.00	372.0
46.10	374.0
47.00	3247.0
48.00	1650.0
49.10	8445.0
50.10	39352.0
51.00	12320.0
52.00	739.0
52.90	313.0
54.30	130.0
55.10	515.0
56.00	2971.0
57.10	5134.0
58.10	349.0
58.90	127.0
60.00	1661.0
61.00	10165.0
62.10	10685.0
63.00	8599.0
64.00	1370.0
65.00	2076.0
65.90	151.0
67.00	775.0
68.00	21064.0
69.00	22432.0
70.00	1398.0
71.20	139.0
72.00	1383.0
73.00	9445.0
74.10	36784.0
75.10	110248.0
76.10	8395.0
77.10	1039.0
77.90	1194.0
78.90	6115.0
80.00	1682.0
81.00	6240.0
82.00	1263.0
86.10	621.0
87.00	8711.0
88.00	10131.0
89.90	153.0
91.00	885.0
92.10	6055.0
93.00	9839.0
94.00	26344.0
95.00	228864.0
96.10	14770.0
97.00	385.0
97.20	378.0
102.90	116.0
103.90	986.0
105.00	378.0
106.00	884.0
106.80	125.0
110.10	222.0
110.80	213.0
112.10	164.0
113.00	165.0
115.00	304.0
116.00	715.0
116.90	1766.0
117.90	740.0
119.00	1607.0
122.90	145.0
123.80	236.0
124.30	147.0
126.00	146.0
127.80	842.0
128.90	484.0
130.00	747.0
131.00	418.0
134.00	127.0
135.00	353.0
136.90	386.0
138.80	173.0
140.10	383.0
141.00	1843.0
141.90	293.0
142.90	3431.0
144.90	1502.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

145.80	346.0
146.80	275.0
147.90	776.0
148.90	161.0
149.70	245.0
150.10	180.0
151.90	161.0
153.00	189.0
154.00	157.0
154.80	569.0
155.90	186.0
156.90	632.0
157.80	114.0
158.80	330.0
160.90	340.0
169.60	153.0
171.00	652.0
172.00	3362.0
174.00	224960.0
175.00	16936.0
176.00	217728.0
177.00	13861.0
177.80	447.0
207.50	111.0
251.80	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
35.20	148.0
36.00	1873.0
37.10	8009.0
38.00	7746.0
39.00	3225.0
40.10	775.0
40.80	225.0
42.10	188.0
43.00	206.0
44.00	1548.0
45.00	1757.0
46.00	305.0
47.00	3029.0
48.00	1409.0
49.10	7762.0
50.10	36016.0
51.00	11417.0
52.00	610.0
52.80	353.0
54.20	147.0
55.10	389.0
56.10	2801.0
57.00	4638.0
58.10	305.0
58.80	128.0
60.00	1514.0
61.00	9170.0
62.10	9983.0
63.00	7628.0
64.00	1060.0
65.10	1876.0
66.00	146.0
67.00	790.0
68.00	18704.0
69.00	20072.0
70.00	1296.0
71.20	146.0
72.00	1295.0
73.00	8420.0
74.10	33040.0
75.10	101112.0
76.10	7554.0
77.10	841.0
77.90	1045.0
78.90	5593.0
80.00	1755.0
81.00	5688.0
82.00	1159.0
82.80	143.0
86.10	561.0
87.00	7638.0
88.00	8651.0
90.00	103.0
91.00	828.0
92.00	5607.0
93.00	8999.0
94.00	23576.0
95.00	209664.0
96.10	13539.0
97.20	388.0
103.10	102.0
103.90	832.0
105.10	292.0
106.00	816.0
106.80	129.0
110.10	214.0
110.90	190.0
112.00	164.0
112.90	152.0
115.00	305.0
115.90	661.0
116.90	1673.0
117.90	614.0
119.00	1303.0
122.10	114.0
123.80	243.0
126.00	178.0
127.90	728.0
128.90	446.0
130.00	734.0
131.00	372.0
135.00	329.0
136.80	348.0
138.80	212.0
140.10	364.0
141.00	1731.0
141.90	375.0
143.00	3144.0
143.80	138.0
144.90	1248.0
145.90	288.0
146.80	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

148.00	737.0
149.00	153.0
149.70	259.0
151.80	160.0
153.10	206.0
153.90	162.0
154.90	542.0
155.90	292.0
156.90	632.0
157.80	140.0
158.80	324.0
161.00	327.0
169.60	104.0
170.90	633.0
172.00	3255.0
174.00	213568.0
175.00	15795.0
176.00	205696.0
177.00	13046.0
177.90	387.0
216.60	112.0
251.80	157.0
268.70	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
35.10	169.0
39.00	126.0
39.90	756.0
40.90	139.0
41.90	136.0
44.00	715.0
50.00	165.0
53.50	122.0
55.00	113.0
57.10	119.0
63.30	102.0
65.00	154.0
71.90	168.0
77.10	133.0
78.10	120.0
78.40	113.0
83.00	107.0
84.80	118.0
99.40	134.0
206.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38