


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112520\
 Data File : VV019436.D
 Acq On : 25 Nov 2020 08:38
 Operator : SY/MD
 Sample : BFB97
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB97

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis
 Last Update : Thu Nov 26 00:24:16 2020

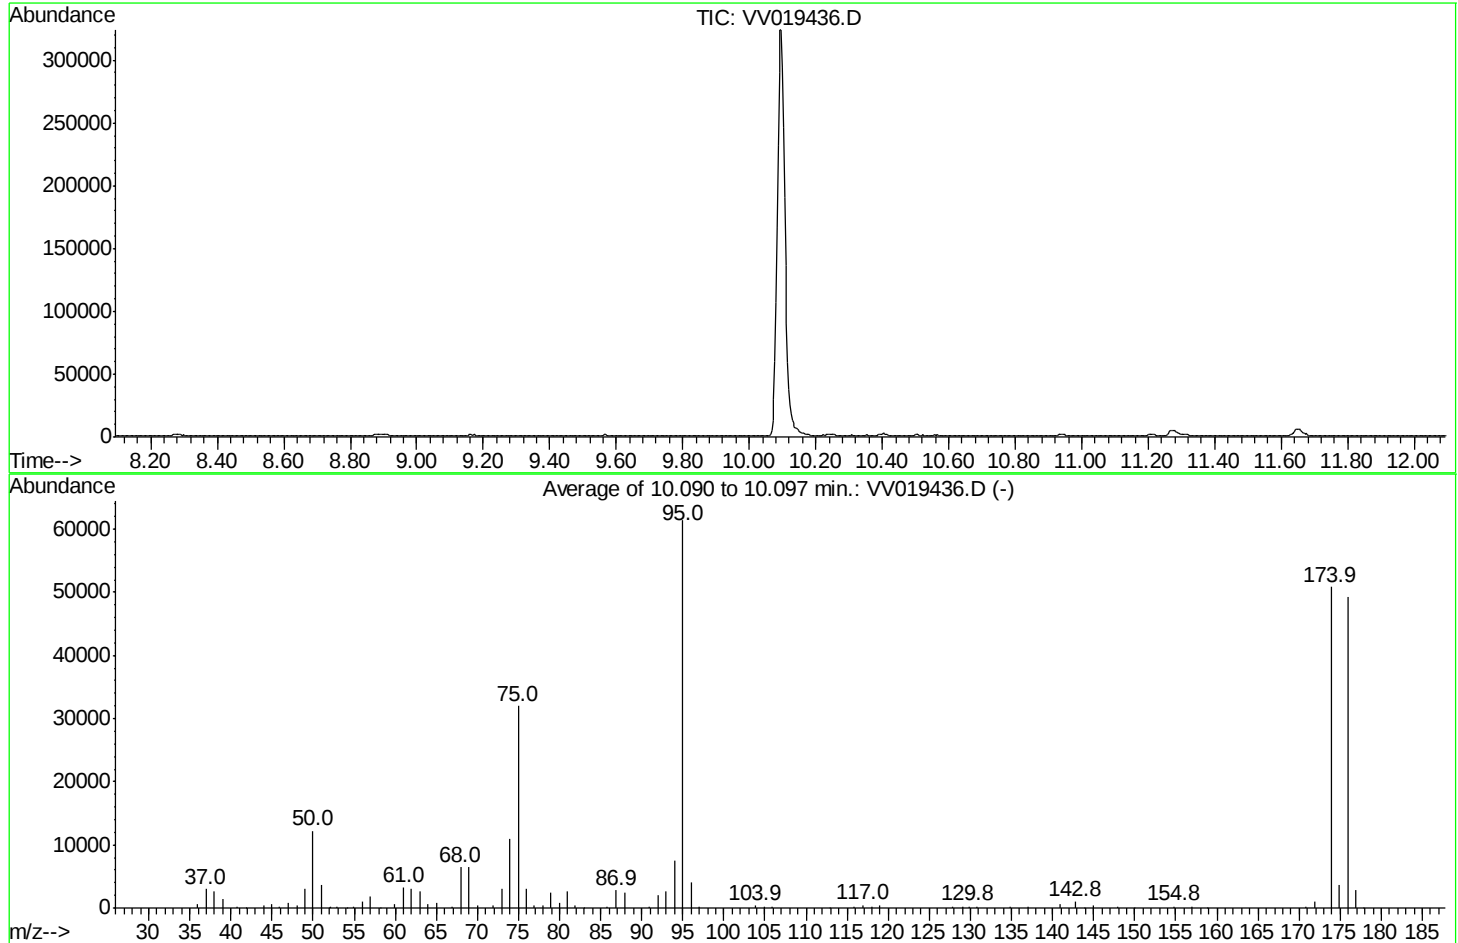

AutoFind: Scans 2799, 2800, 2801; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12166	PASS
75	95	30	80	52.1	31986	PASS
95	95	100	100	100.0	61394	PASS
96	95	5	9	6.5	4004	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.8	50858	PASS
175	174	5	9	7.3	3714	PASS
176	174	95	101	96.8	49226	PASS
177	176	5	9	6.0	2929	PASS

Scan 2789 (10.058 min): VV019436.D
BFB97

m/z	Abundance
39.90	346.0
44.00	489.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
35.90	603.0
37.00	2621.0
38.00	2543.0
39.00	1336.0
39.90	316.0
40.70	104.0
41.90	113.0
44.00	895.0
45.00	550.0
45.90	192.0
47.00	793.0
48.00	477.0
49.00	2961.0
50.00	11470.0
51.00	3480.0
51.90	206.0
52.10	190.0
52.90	158.0
54.90	280.0
56.00	822.0
57.00	1747.0
60.00	596.0
61.00	3059.0
62.00	2965.0
63.00	2565.0
64.00	532.0
65.00	867.0
67.00	277.0
68.00	5819.0
69.00	6176.0
70.00	503.0
71.90	420.0
73.00	2924.0
74.00	10219.0
75.00	30144.0
76.00	2939.0
76.90	413.0
77.90	366.0
78.90	2245.0
80.00	693.0
80.90	2431.0
81.90	493.0
82.90	121.0
85.70	103.0
86.90	2539.0
87.90	2361.0
90.90	283.0
92.00	1803.0
93.00	2338.0
94.00	6946.0
95.00	58112.0
96.00	3798.0
97.00	180.0
104.00	322.0
104.90	131.0
105.90	237.0
112.90	106.0
115.80	253.0
117.00	483.0
117.90	318.0
119.00	332.0
127.70	207.0
129.10	135.0
129.80	251.0
130.90	116.0
134.80	144.0
137.00	111.0
140.90	489.0
142.90	956.0
144.90	319.0
147.90	161.0
154.80	255.0
156.90	153.0
170.90	159.0
171.90	855.0
173.90	45768.0
174.90	3389.0
175.90	44528.0
176.90	2644.0
177.80	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
36.00	676.0
37.00	3051.0
38.00	2710.0
39.10	1432.0
39.90	324.0
40.70	108.0
41.90	113.0
44.00	873.0
45.00	636.0
46.00	236.0
47.00	837.0
48.00	470.0
49.00	3162.0
50.00	12604.0
51.00	3842.0
52.00	214.0
52.90	168.0
54.90	279.0
56.00	1045.0
57.00	1838.0
59.90	669.0
61.00	3294.0
62.00	3253.0
63.00	2758.0
64.00	572.0
65.00	925.0
66.90	309.0
68.00	6605.0
69.00	6737.0
70.00	515.0
71.90	413.0
73.00	3141.0
74.00	11316.0
75.00	33184.0
76.00	3156.0
76.90	385.0
77.90	424.0
78.90	2600.0
80.00	758.0
80.90	2733.0
81.90	512.0
82.90	111.0
85.70	133.0
86.90	2949.0
87.90	2617.0
90.80	299.0
92.00	2094.0
93.00	2735.0
94.00	7937.0
95.00	63248.0
96.00	4077.0
97.00	188.0
103.90	312.0
104.80	166.0
105.90	285.0
112.90	103.0
115.80	291.0
117.00	450.0
117.90	330.0
118.90	342.0
127.70	248.0
129.10	138.0
129.80	288.0
130.80	138.0
134.80	166.0
137.00	121.0
140.90	686.0
142.90	1032.0
145.00	372.0
147.90	178.0
149.90	106.0
154.80	256.0
156.90	158.0
158.80	104.0
170.80	160.0
171.90	1017.0
173.90	52784.0
174.90	3792.0
175.90	51112.0
176.90	3044.0
177.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
36.00	737.0
37.00	3185.0
38.00	2676.0
39.10	1336.0
39.90	371.0
40.80	114.0
44.00	758.0
45.00	693.0
46.00	232.0
47.00	763.0
48.00	456.0
49.00	2999.0
50.00	12424.0
51.00	3790.0
52.00	217.0
52.80	169.0
54.10	107.0
55.00	226.0
56.00	1161.0
57.00	1793.0
58.20	105.0
59.90	678.0
61.00	3143.0
62.00	3188.0
63.00	2883.0
64.00	572.0
65.00	868.0
67.00	284.0
68.00	6774.0
69.00	6536.0
70.00	473.0
72.00	351.0
73.00	3111.0
74.00	11312.0
75.00	32632.0
76.00	3041.0
76.90	384.0
77.90	334.0
78.90	2578.0
79.90	703.0
80.90	2700.0
81.90	527.0
85.70	145.0
86.90	2996.0
87.90	2590.0
90.80	237.0
92.00	2128.0
93.00	2934.0
94.00	7931.0
95.00	62824.0
96.00	4137.0
97.00	139.0
103.80	315.0
104.80	162.0
105.90	297.0
115.80	286.0
116.90	452.0
118.00	270.0
118.90	374.0
127.80	239.0
129.00	130.0
129.80	297.0
130.80	138.0
134.90	201.0
137.00	143.0
140.90	775.0
142.80	1010.0
143.80	129.0
145.00	425.0
147.90	222.0
154.80	174.0
156.90	146.0
158.90	129.0
170.80	154.0
171.90	1026.0
173.90	54024.0
174.90	3962.0
175.90	52040.0
176.90	3099.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97