

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112522\
 Data File : VW029351.D
 Acq On : 25 Nov 2022 13:22
 Operator : SY/MD
 Sample : VIBLK234
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK234

Quant Time: Nov 25 21:31:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 25 21:27:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	297765	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	262856	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	133203	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	93107	5.081	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.600%
7) Chloroethane-d5	1.564	69	72189	5.382	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.600%
11) 1,1-Dichloroethene-d2	2.105	63	111048	3.787	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.800%
20) 2-Butanone-d5	3.896	46	183687	59.922	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.840%
24) Chloroform-d	4.339	84	164326	5.024	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.024	65	78314	5.442	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.800%
32) Benzene-d6	5.043	84	368545	5.073	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.400%
36) 1,2-Dichloropropane-d6	6.063	67	109298	5.354	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.000%
41) Toluene-d8	7.307	98	336445	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
43) trans-1,3-Dichloroprop...	7.616	79	40388	5.132	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.600%
46) 2-Hexanone-d5	8.085	63	143883	51.287	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.580%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	72567	5.761	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.200%
66) 1,2-Dichlorobenzene-d4	11.612	152	123275	5.298	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%
Target Compounds						
					Qvalue	
3) Chloromethane	1.243	50	9011	0.443	ug/L	98
16) Methylene chloride	2.503	84	38426	1.643	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029351.D
Acq On : 25 Nov 2022 13:22
Operator : SY/MD
Sample : VIBLK234
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK234

Quant Time: Nov 25 21:31:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 25 21:27:54 2022
Response via : Initial Calibration




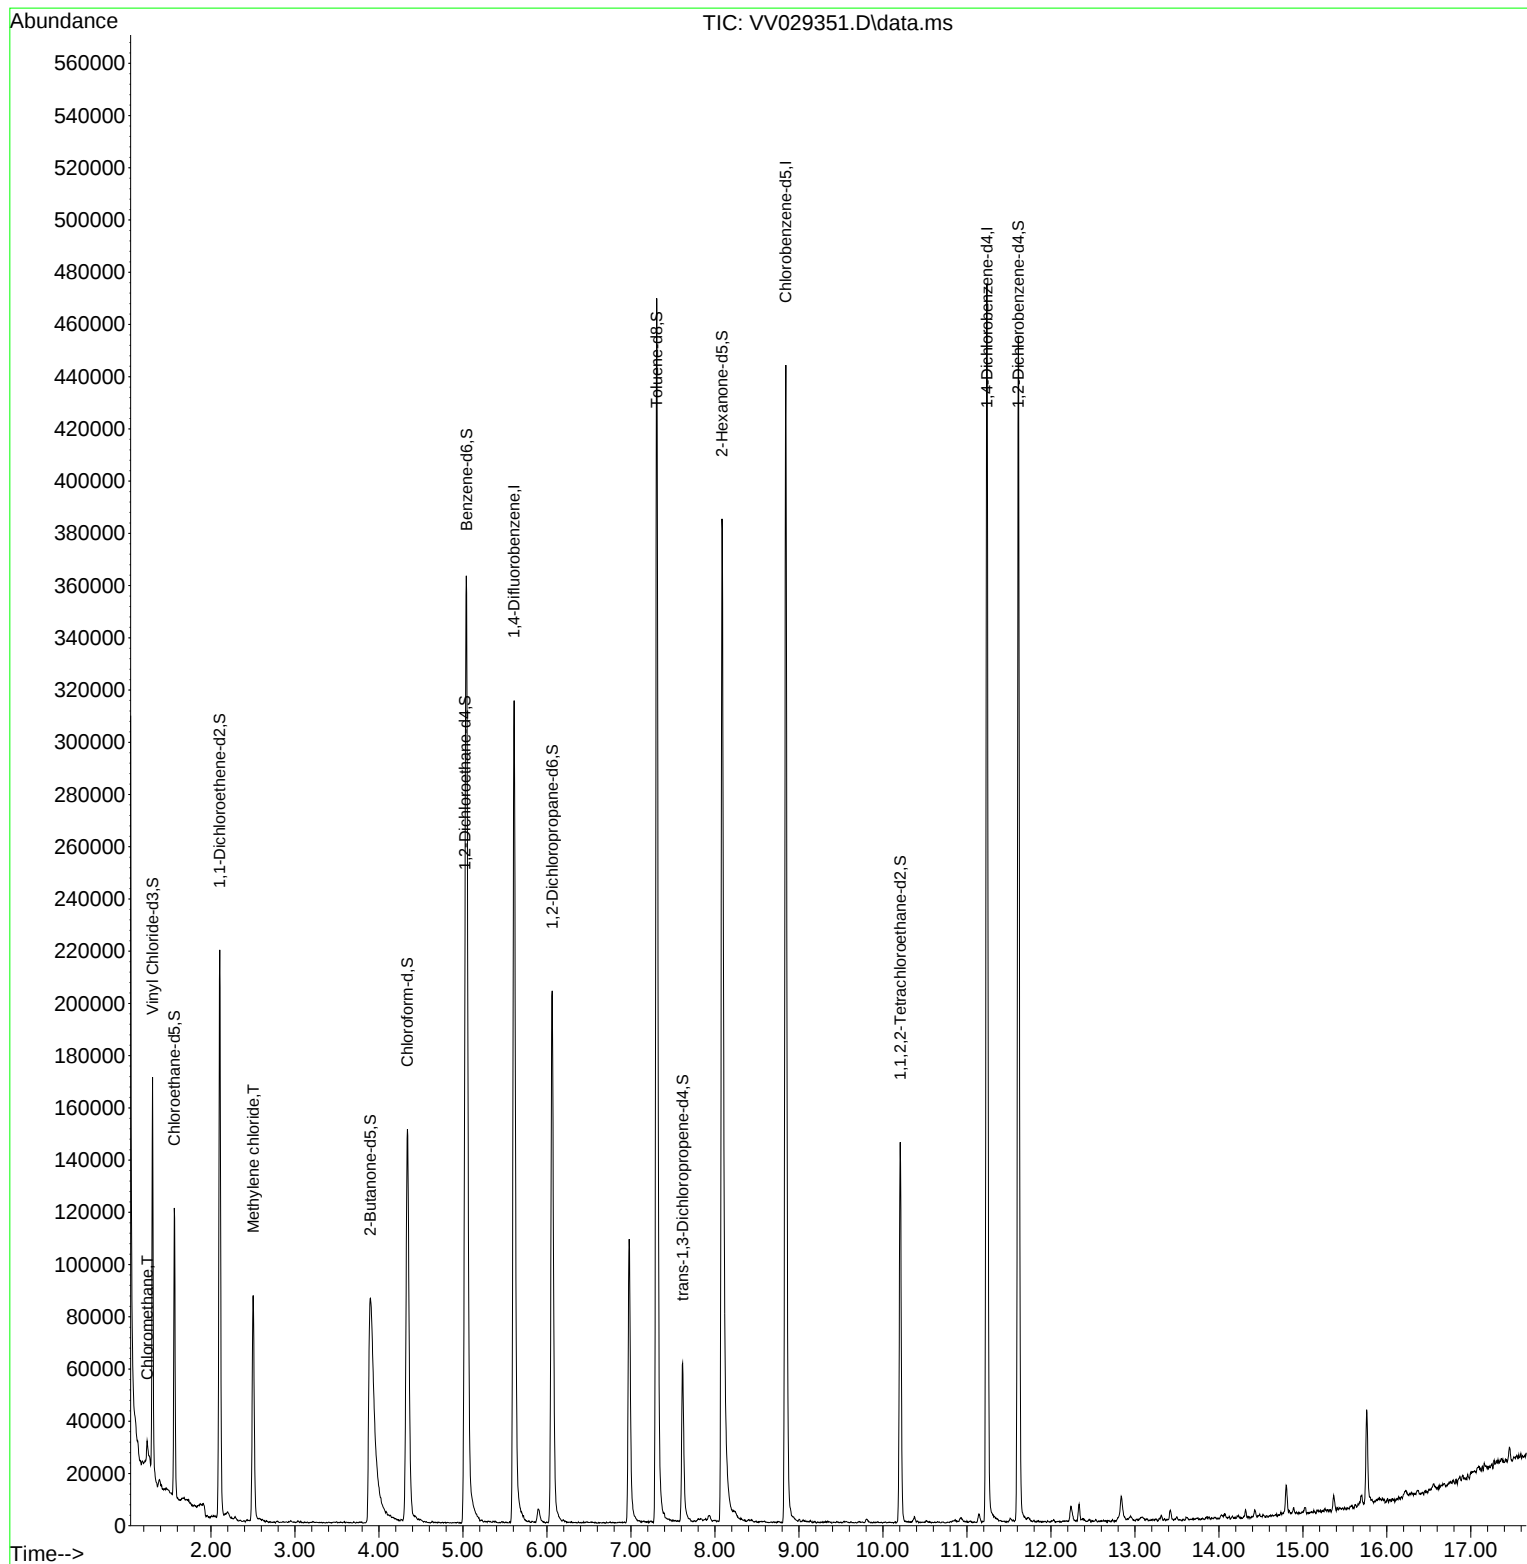


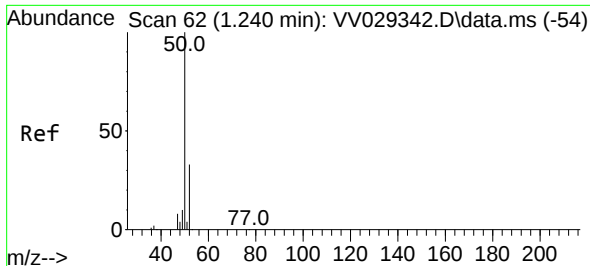

#3
Chloromethane
Concen: 0.443 ug/L
RT: 1.243 min Scan# 61
Delta R.T. 0.003 min
Lab File: VV029351.D
Acq: 25 Nov 2022 13:22

Instrument :
MSVOA_V
ClientSampleId :
VIBLK234

Tgt Ion: 50 Resp: 9011
Ion Ratio Lower Upper
50 100
52 34.4 23.2 43.2

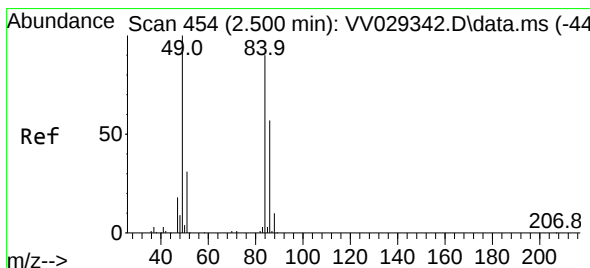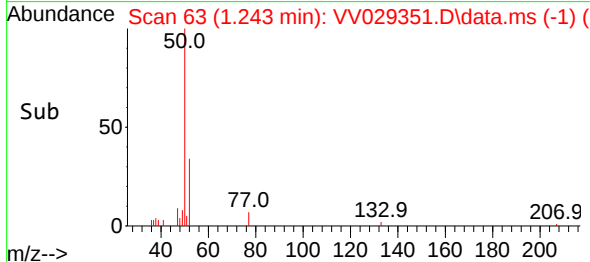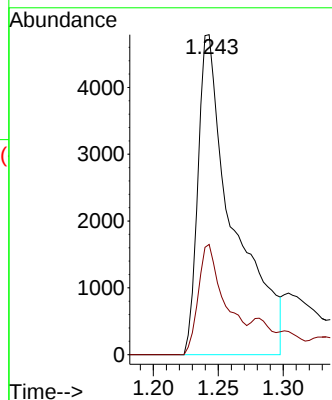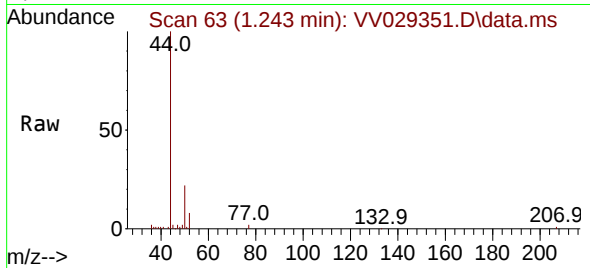

#16
Methylene chloride
Concen: 1.643 ug/L
RT: 2.503 min Scan# 455
Delta R.T. 0.003 min
Lab File: VV029351.D
Acq: 25 Nov 2022 13:22

Tgt Ion: 84 Resp: 38426
Ion Ratio Lower Upper
84 100
86 63.2 45.6 84.6
49 111.7 77.8 144.4

