

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112522\
 Data File : VW029354.D
 Acq On : 25 Nov 2022 14:33
 Operator : SY/MD
 Sample : N5725-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB69

Quant Time: Nov 25 21:31:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 25 21:27:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	313025	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	277278	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	141135	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	87467	4.541	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.800%	
7) Chloroethane-d5	1.565	69	67998	4.822	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.400%	
11) 1,1-Dichloroethene-d2	2.105	63	104278	3.383	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.892	46	171942	53.356	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.720%	
24) Chloroform-d	4.339	84	157946	4.594	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.800%	
26) 1,2-Dichloroethane-d4	5.024	65	74036	4.894	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.800%	
32) Benzene-d6	5.043	84	350787	4.578	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	6.063	67	104873	4.870	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.400%	
41) Toluene-d8	7.307	98	318455	4.403	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.000%	
43) trans-1,3-Dichloroprop...	7.616	79	37172	4.477	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.600%	
46) 2-Hexanone-d5	8.085	63	140944	47.627	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.260%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	69306	5.216	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4	11.612	152	120060	4.869	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.400%	
Target Compounds						
13) Acetone	2.182	43	10329	4.408	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029354.D
Acq On : 25 Nov 2022 14:33
Operator : SY/MD
Sample : N5725-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB69

Quant Time: Nov 25 21:31:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 25 21:27:54 2022
Response via : Initial Calibration

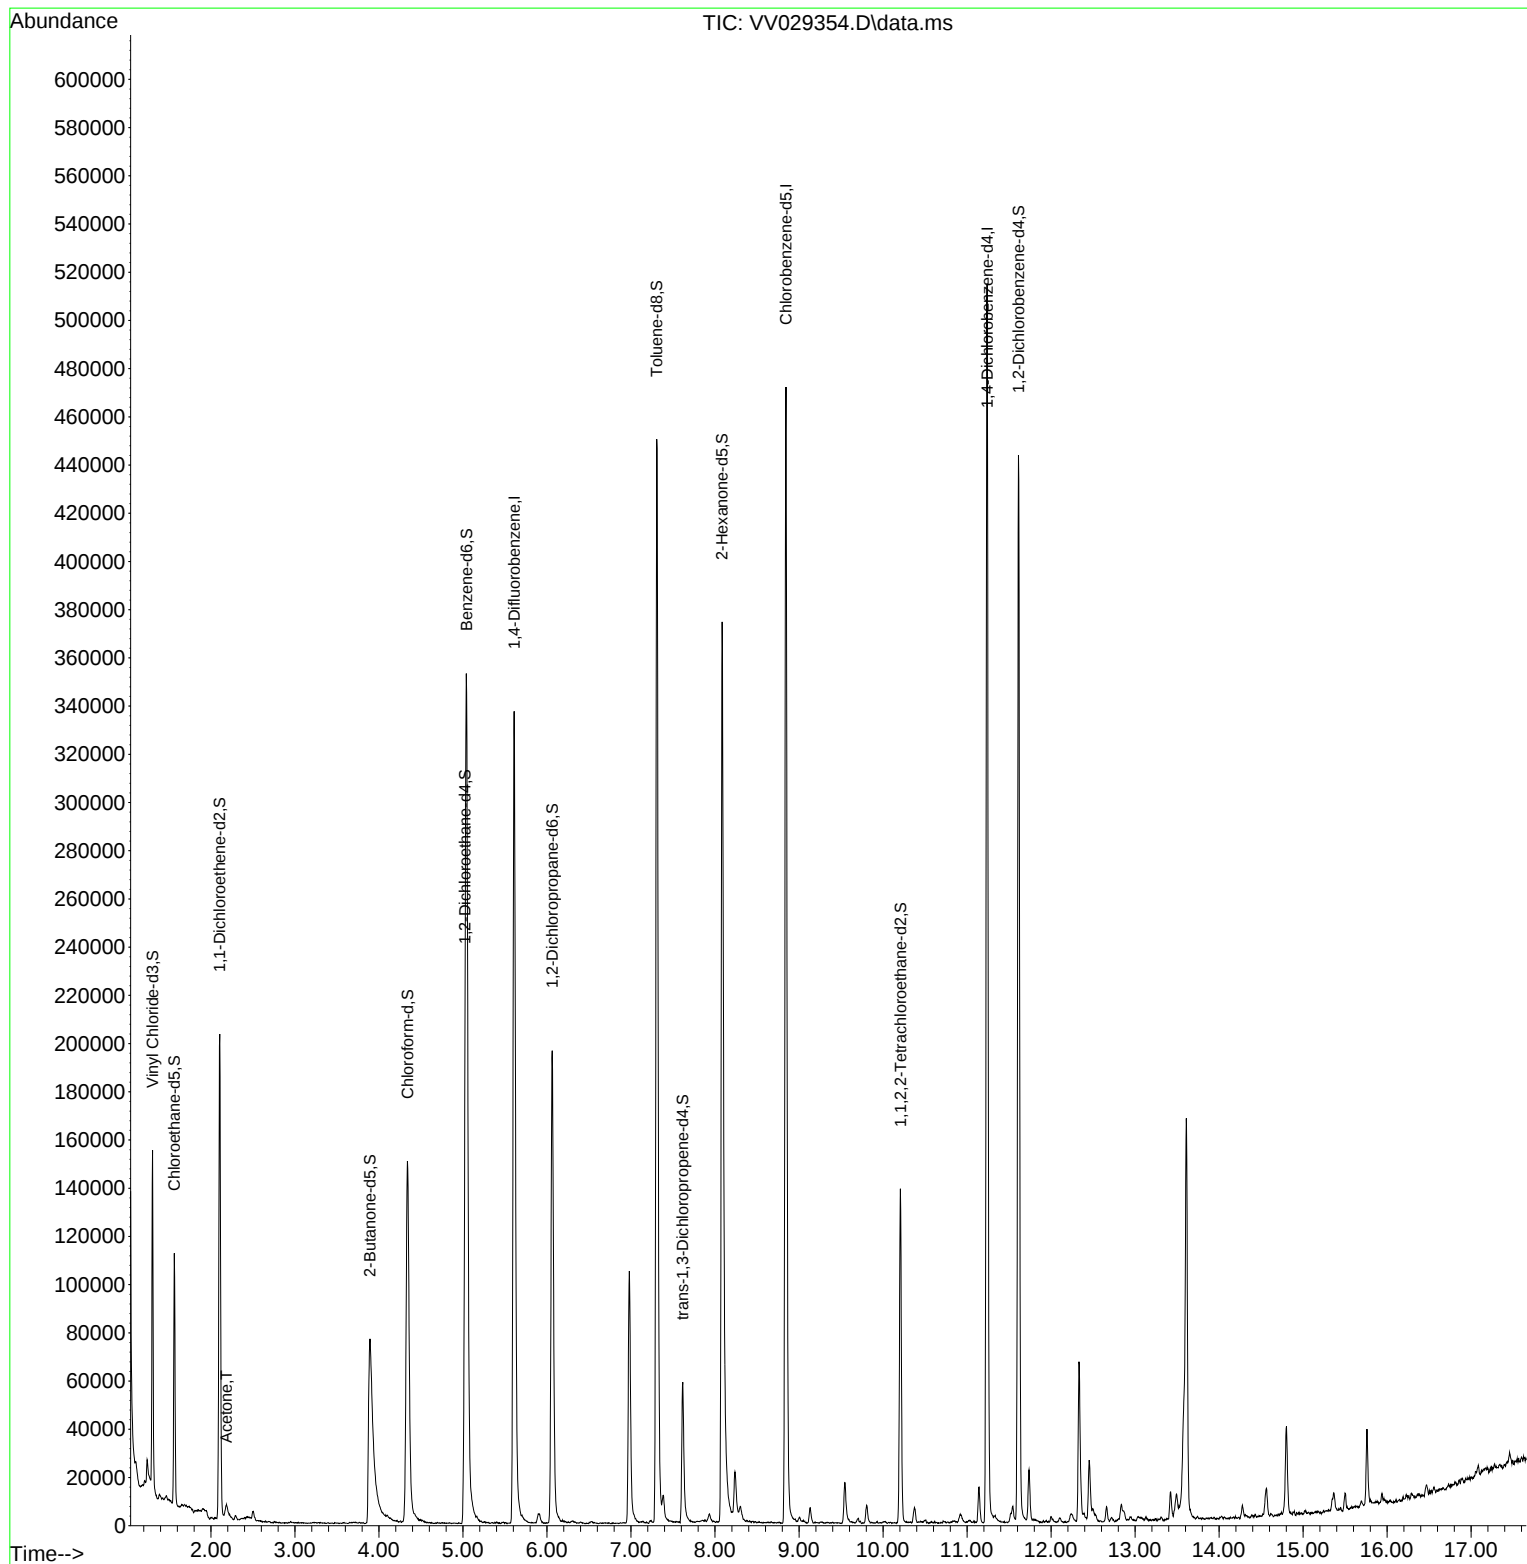

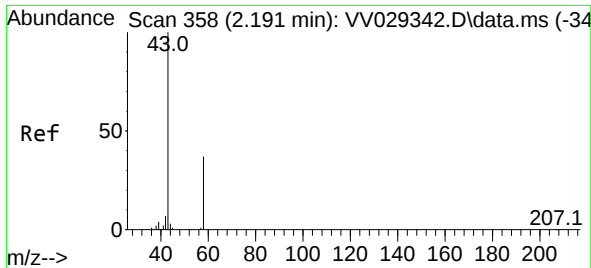

#13
 Acetone
 Concen: 4.408 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV029354.D
 Acq: 25 Nov 2022 14:33

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB69

Tgt Ion: 43 Resp: 10329
 Ion Ratio Lower Upper
 43 100
 58 30.5 0.0 70.8

