

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112522\
 Data File : VW029355.D
 Acq On : 25 Nov 2022 14:58
 Operator : SY/MD
 Sample : N5725-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB70

Quant Time: Nov 25 21:32:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 25 21:27:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	325824	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	286647	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	139320	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	83381	4.158	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.200%
7) Chloroethane-d5	1.564	69	67254	4.582	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.101	63	103119	3.214	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.200%
20) 2-Butanone-d5	3.899	46	169360	50.490	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.980%
24) Chloroform-d	4.339	84	155912	4.356	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
26) 1,2-Dichloroethane-d4	5.024	65	73712	4.681	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
32) Benzene-d6	5.043	84	339440	4.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.063	67	101903	4.578	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.600%
41) Toluene-d8	7.307	98	312849	4.184	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
43) trans-1,3-Dichloroprop...	7.616	79	36528	4.256	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.085	63	141359	46.206	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.420%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	66760	4.860	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.612	152	113114	4.648	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.000%
Target Compounds						
					Qvalue	
13) Acetone	2.195	43	10137	4.156	ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029355.D
Acq On : 25 Nov 2022 14:58
Operator : SY/MD
Sample : N5725-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB70

Quant Time: Nov 25 21:32:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 25 21:27:54 2022
Response via : Initial Calibration

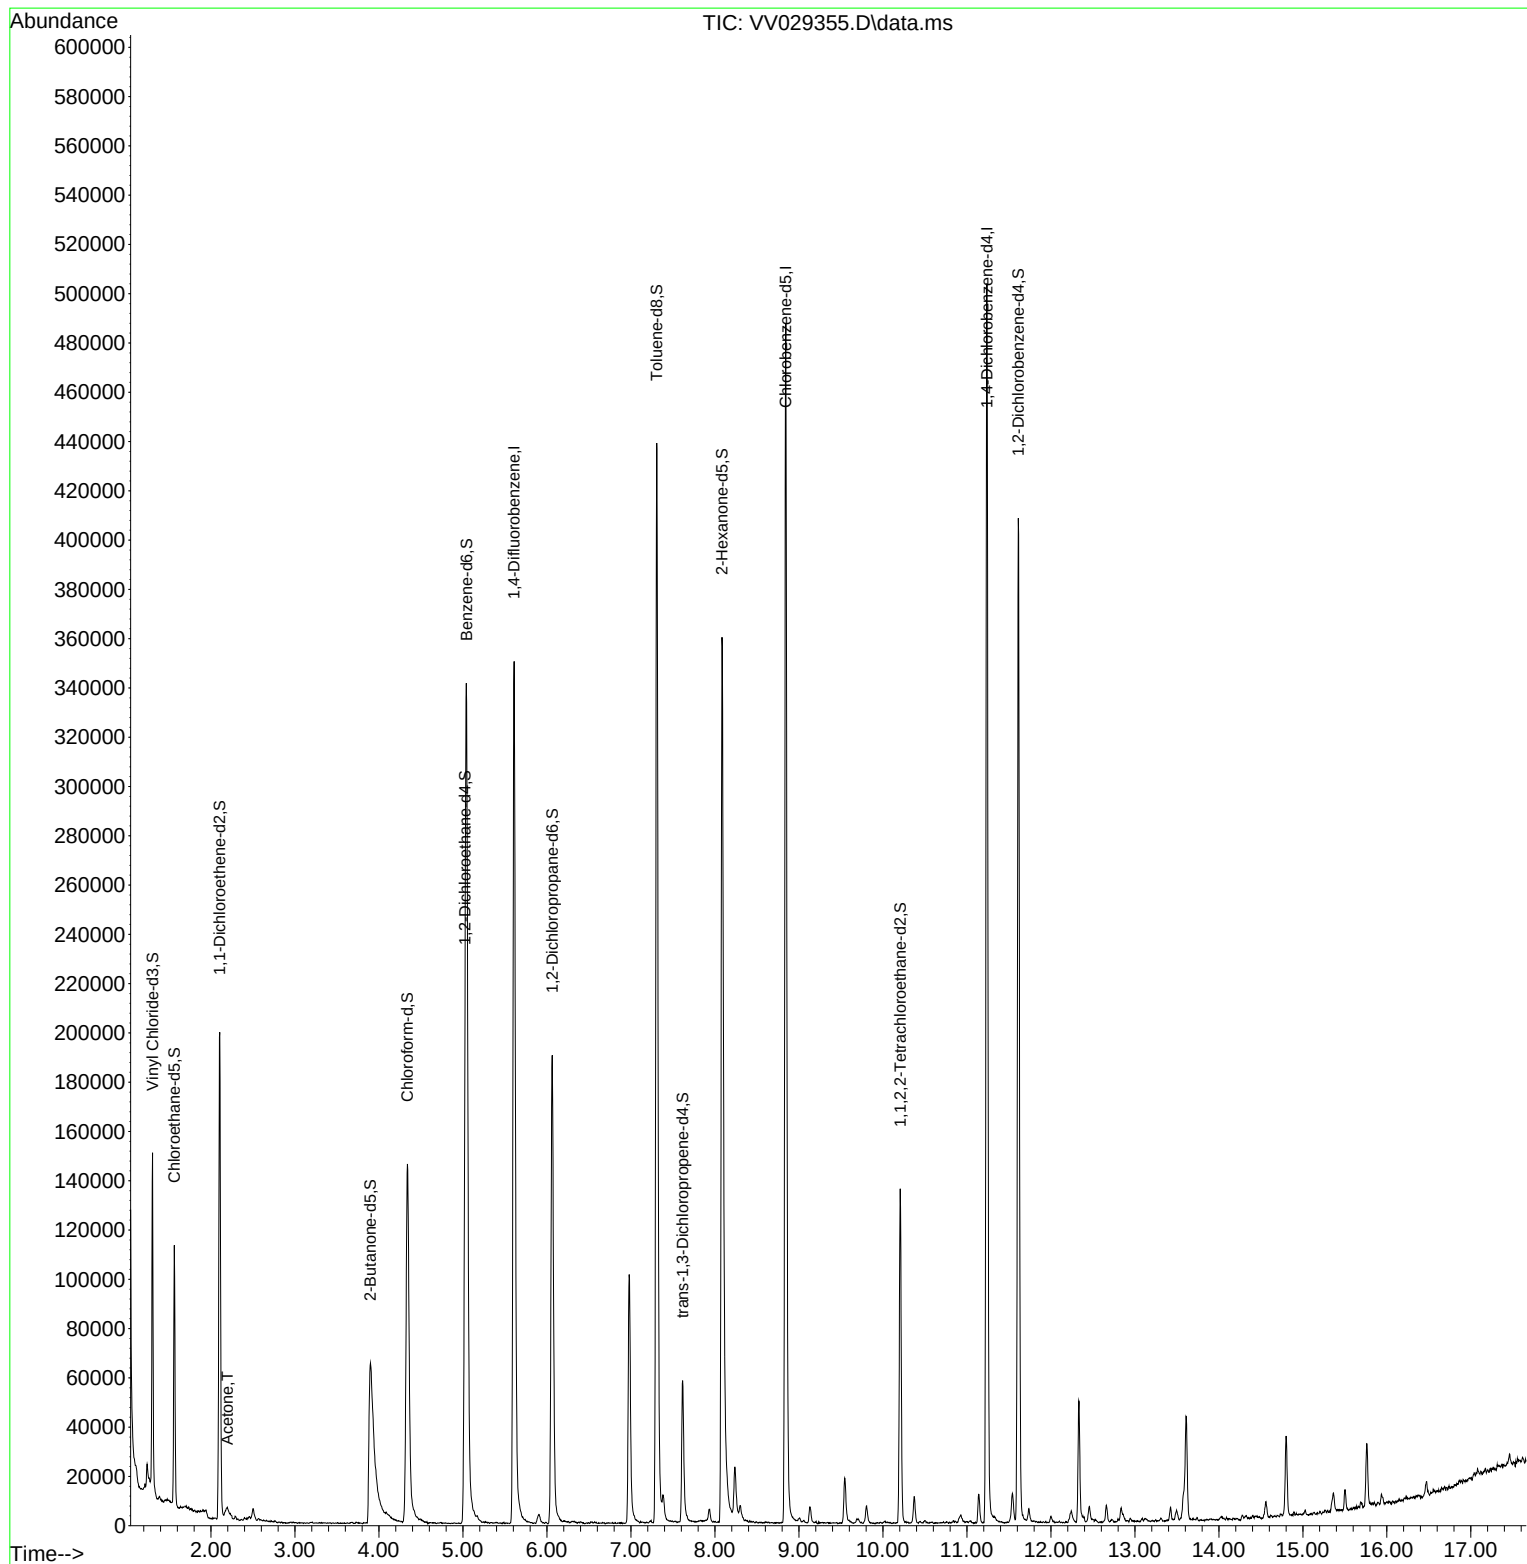

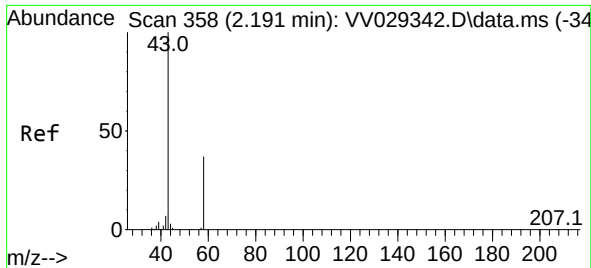

#13

Acetone

Concen: 4.156 ug/L

RT: 2.195 min Scan# 3

Delta R.T. 0.003 min

Lab File: VV029355.D


Acq: 25 Nov 2022 14:58

Instrument :

MSVOA_V

ClientSampleId :

BHB70

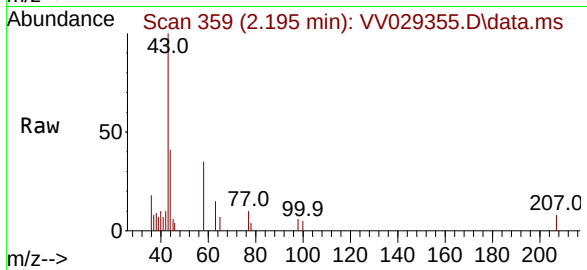

Tgt Ion: 43 Resp: 10137

Ion Ratio Lower Upper

43 100

58 20.7 0.0 70.8

