

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029359.D
 Acq On : 25 Nov 2022 16:36
 Operator : SY/MD
 Sample : N5770-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M9

Quant Time: Nov 25 21:32:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 25 21:27:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	293487	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	260852	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	126447	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	87229	4.830	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.600%
7) Chloroethane-d5	1.564	69	66227	5.009	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.200%
11) 1,1-Dichloroethene-d2	2.105	63	104924	3.630	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	3.889	46	169769	56.189	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.380%
24) Chloroform-d	4.339	84	156785	4.863	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.024	65	73722	5.197	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	5.043	84	340553	4.724	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
36) 1,2-Dichloropropane-d6	6.063	67	103505	5.109	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%
41) Toluene-d8	7.310	98	317080	4.660	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
43) trans-1,3-Dichloroprop...	7.616	79	36084	4.620	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.400%
46) 2-Hexanone-d5	8.085	63	144896	52.045	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.100%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	69617	5.569	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.400%
66) 1,2-Dichlorobenzene-d4	11.615	152	115096	5.210	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.200%
Target Compounds					Qvalue	
13) Acetone	2.182	43	37995	17.295	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029359.D
Acq On : 25 Nov 2022 16:36
Operator : SY/MD
Sample : N5770-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M9

Quant Time: Nov 25 21:32:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 25 21:27:54 2022
Response via : Initial Calibration

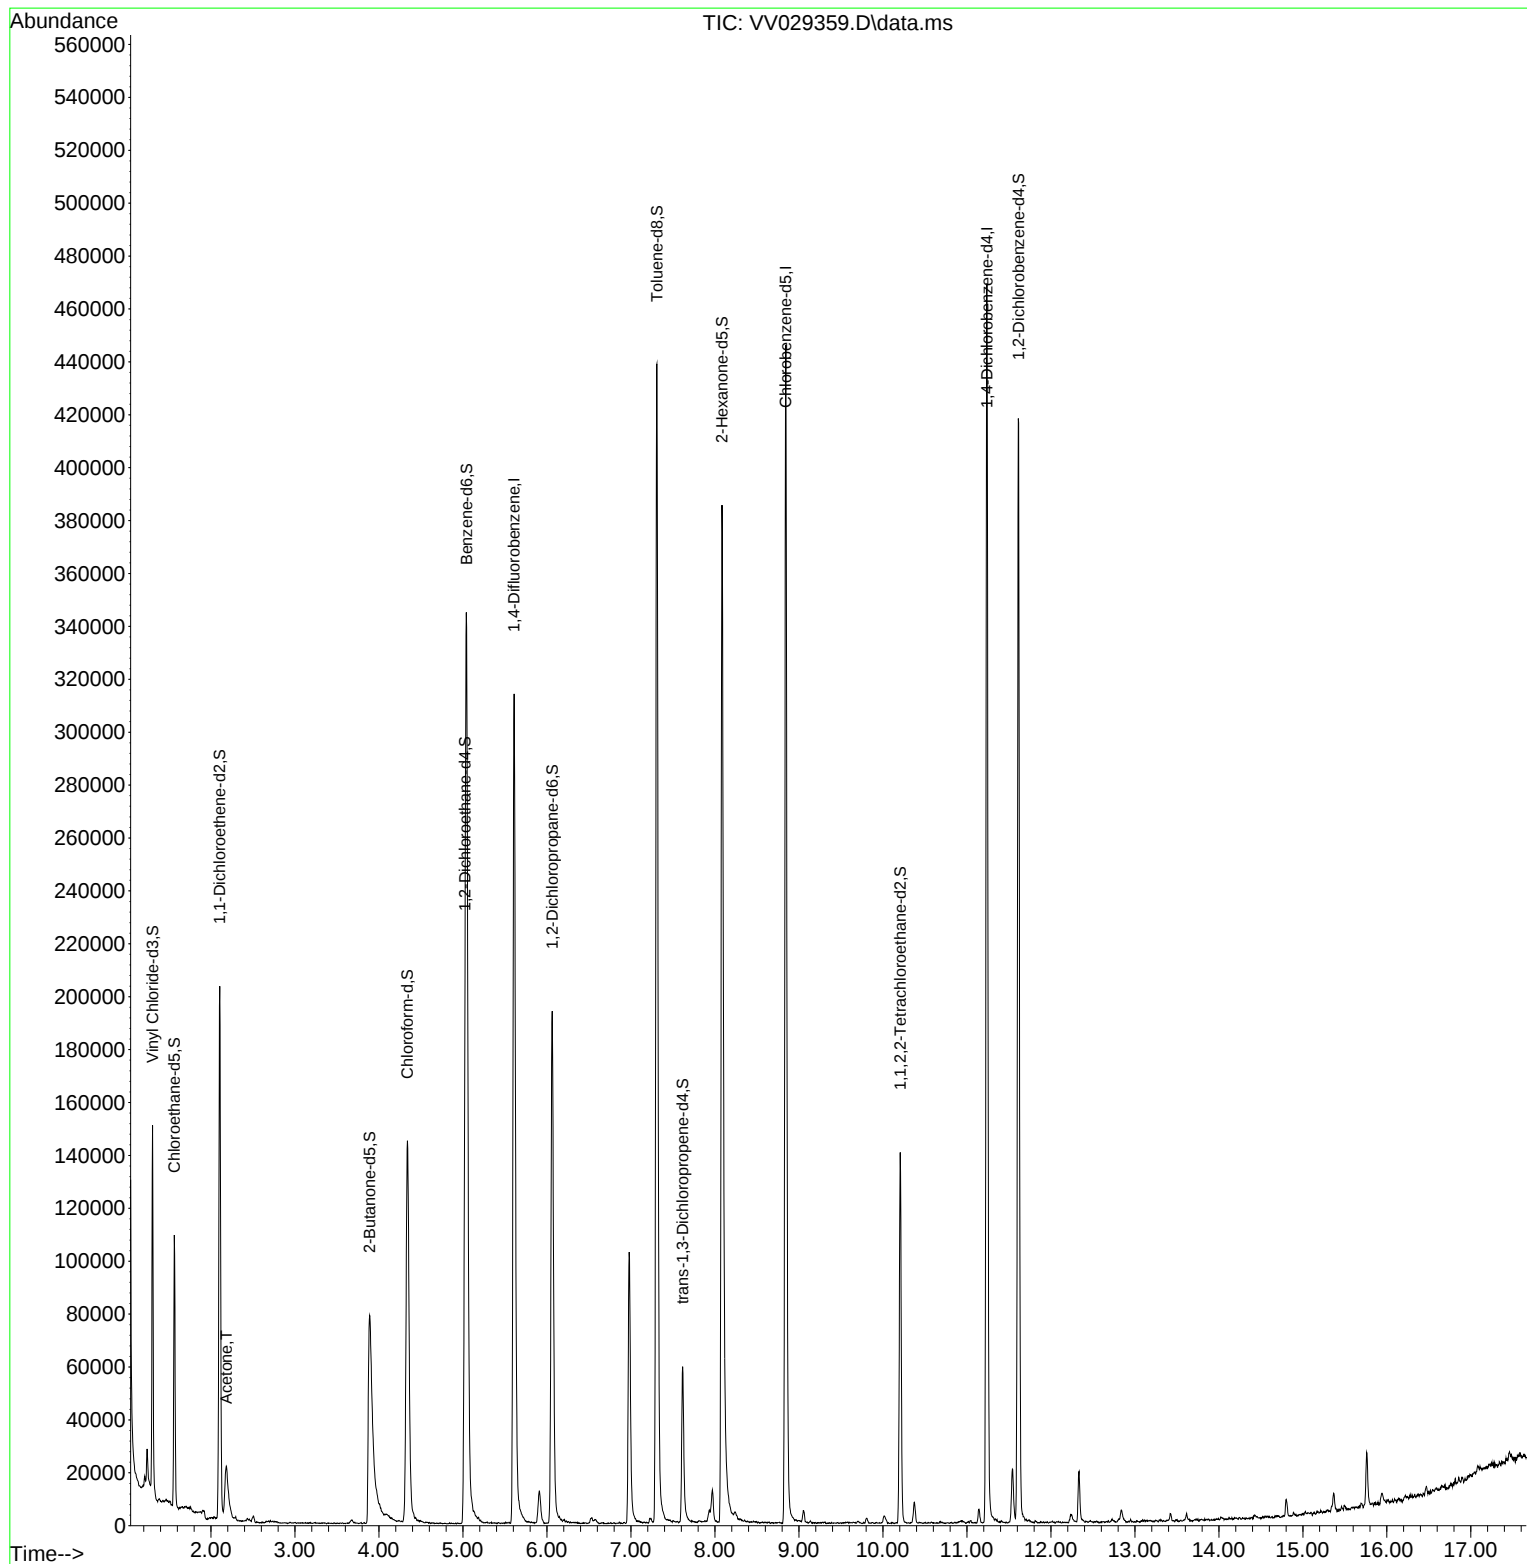

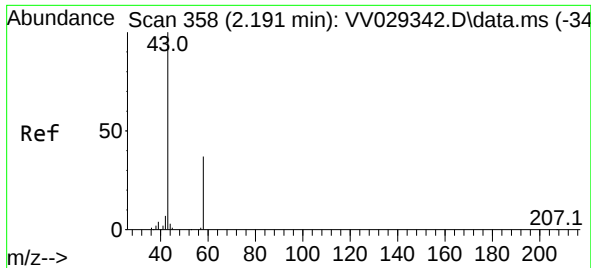

#13
 Acetone
 Concen: 17.295 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV029359.D
 Acq: 25 Nov 2022 16:36

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M9

Tgt Ion: 43 Resp: 37995
 Ion Ratio Lower Upper
 43 100
 58 36.3 0.0 70.8

