

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112522\
 Data File : VW029360.D
 Acq On : 25 Nov 2022 17:01
 Operator : SY/MD
 Sample : N5770-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1N0

Quant Time: Nov 25 21:33:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 25 21:27:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	287190	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	253334	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	130967	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	86334	4.885	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.600%
7) Chloroethane-d5	1.564	69	65916	5.095	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.800%
11) 1,1-Dichloroethene-d2	2.105	63	98617	3.487	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.800%
20) 2-Butanone-d5	3.892	46	165301	55.909	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.820%
24) Chloroform-d	4.339	84	149088	4.726	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
26) 1,2-Dichloroethane-d4	5.027	65	70458	5.076	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.043	84	334509	4.778	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	6.063	67	97963	4.979	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.307	98	304107	4.602	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	7.616	79	37568	4.953	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.000%
46) 2-Hexanone-d5	8.085	63	141386	52.292	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.580%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	65998	5.436	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.800%
66) 1,2-Dichlorobenzene-d4	11.612	152	114591	5.008	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.200%
Target Compounds					Qvalue	
13) Acetone	2.185	43	36027	16.759	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029360.D
Acq On : 25 Nov 2022 17:01
Operator : SY/MD
Sample : N5770-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1N0


Quant Time: Nov 25 21:33:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 25 21:27:54 2022
Response via : Initial Calibration

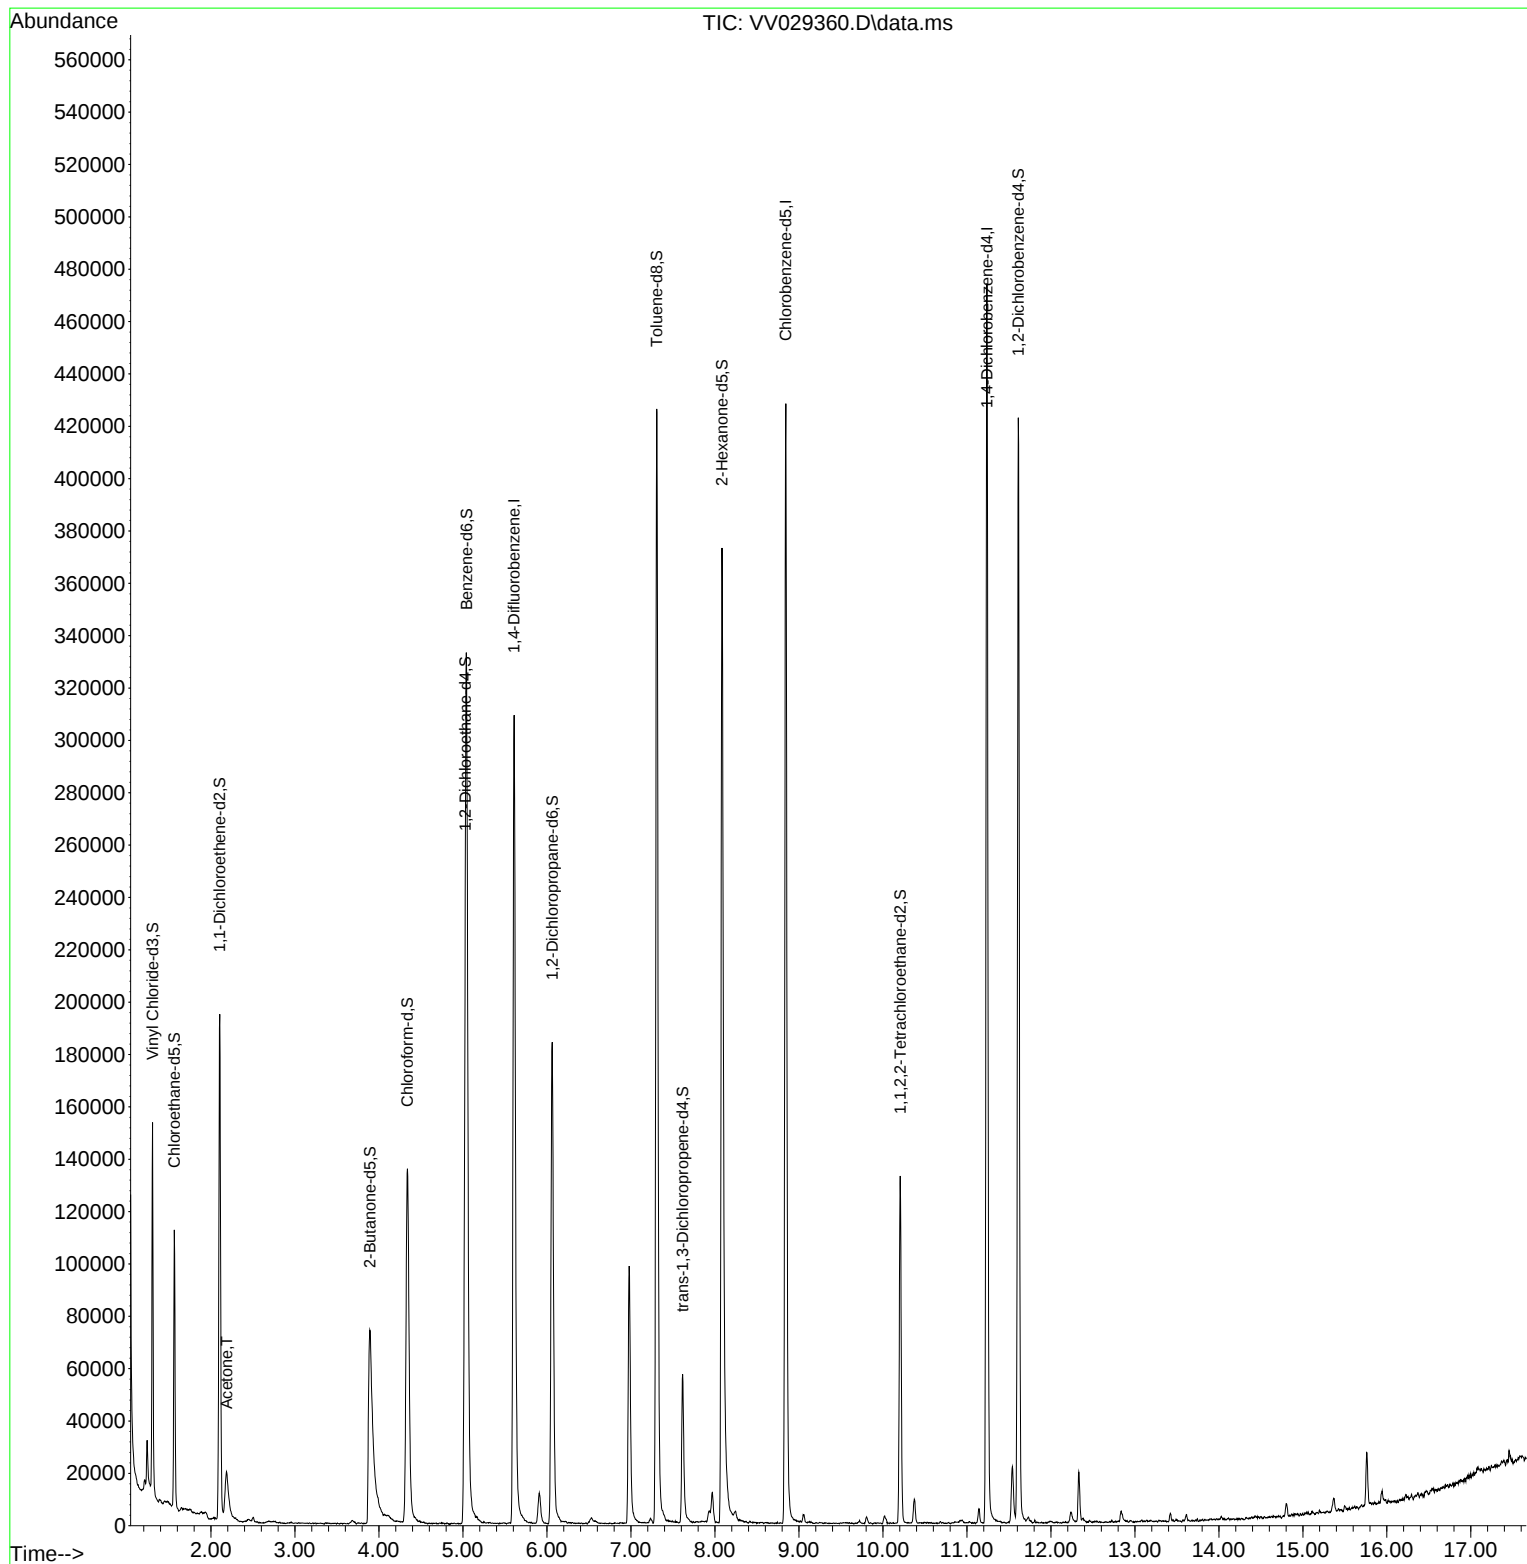

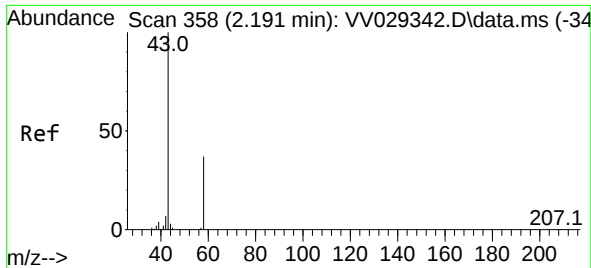

#13
 Acetone
 Concen: 16.759 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV029360.D
 Acq: 25 Nov 2022 17:01

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1N0

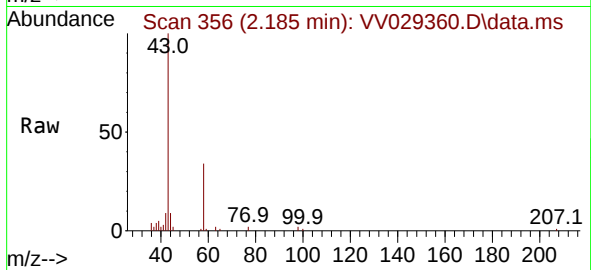

Tgt Ion: 43 Resp: 36027
 Ion Ratio Lower Upper
 43 100
 58 32.5 0.0 70.8

