

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW112522\  
 Data File : VW029361.D  
 Acq On : 25 Nov 2022 17:26  
 Operator : SY/MD  
 Sample : N5770-09  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BH1N1

Quant Time: Nov 25 21:33:18 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112322WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 25 21:27:54 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min)  |
|-------------------------------|--------|-------|----------|----------|-------|-----------|
| -----                         |        |       |          |          |       |           |
| Internal Standards            |        |       |          |          |       |           |
| 1) 1,4-Difluorobenzene        | 5.609  | 114   | 297990   | 5.000    | ug/L  | 0.00      |
| 28) Chlorobenzene-d5          | 8.844  | 117   | 266861   | 5.000    | ug/L  | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.239 | 152   | 135101   | 5.000    | ug/L  | 0.00      |
| System Monitoring Compounds   |        |       |          |          |       |           |
| 4) Vinyl Chloride-d3          | 1.304  | 65    | 85823    | 4.680    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 93.600%   |
| 7) Chloroethane-d5            | 1.564  | 69    | 67176    | 5.004    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 100.000%  |
| 11) 1,1-Dichloroethene-d2     | 2.105  | 63    | 102880   | 3.506    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 70.200%   |
| 20) 2-Butanone-d5             | 3.896  | 46    | 172407   | 56.199   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 112.400%  |
| 24) Chloroform-d              | 4.339  | 84    | 154465   | 4.719    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 94.400%   |
| 26) 1,2-Dichloroethane-d4     | 5.024  | 65    | 73643    | 5.113    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 102.200%  |
| 32) Benzene-d6                | 5.043  | 84    | 343402   | 4.656    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 93.200%   |
| 36) 1,2-Dichloropropane-d6    | 6.063  | 67    | 101831   | 4.914    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 98.200%   |
| 41) Toluene-d8                | 7.310  | 98    | 314597   | 4.519    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 90.400%   |
| 43) trans-1,3-Dichloroprop... | 7.616  | 79    | 37559    | 4.701    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 94.000%   |
| 46) 2-Hexanone-d5             | 8.085  | 63    | 149602   | 52.526   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 105.060%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.207 | 84    | 69738    | 5.453    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 109.000%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.612 | 152   | 118332   | 5.014    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 100.200%  |
| Target Compounds              |        |       |          |          |       |           |
| 13) Acetone                   | 2.188  | 43    | 36171    | 16.216   | ug/L  | Qvalue 99 |
| -----                         |        |       |          |          |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112522\  
Data File : VV029361.D  
Acq On : 25 Nov 2022 17:26  
Operator : SY/MD  
Sample : N5770-09  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BH1N1

Quant Time: Nov 25 21:33:18 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112322WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Nov 25 21:27:54 2022  
Response via : Initial Calibration

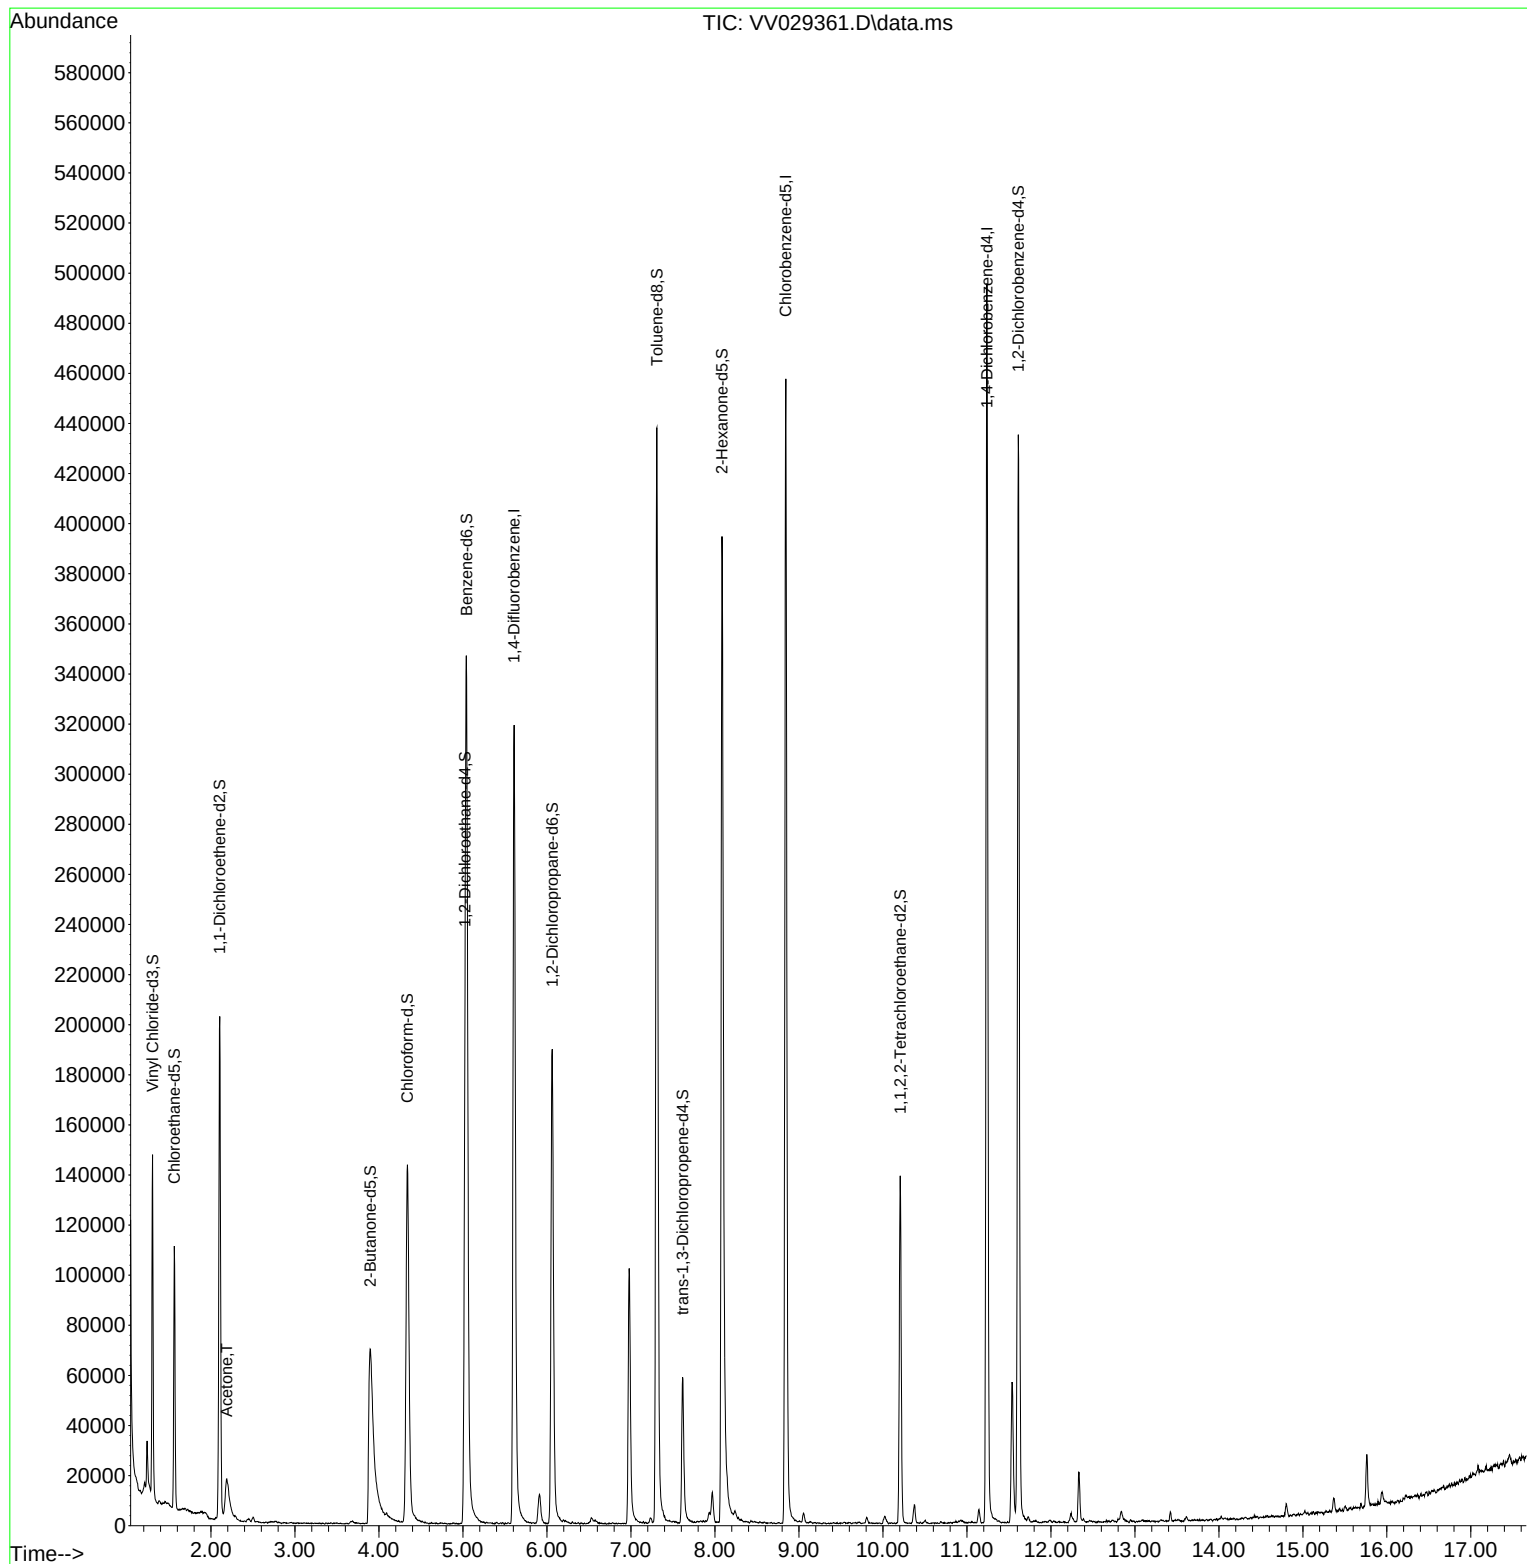

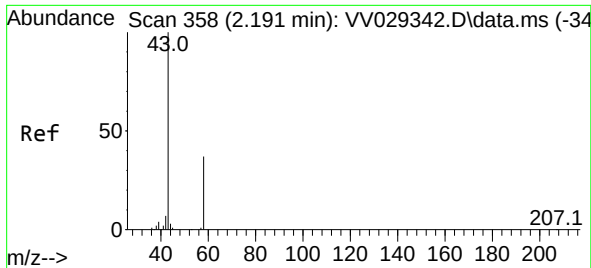

#13

Acetone

Concen: 16.216 ug/L

RT: 2.188 min Scan# 3

Delta R.T. -0.003 min

Lab File: VV029361.D


Acq: 25 Nov 2022 17:26

Instrument :

MSVOA\_V

ClientSampleId :

BH1N1

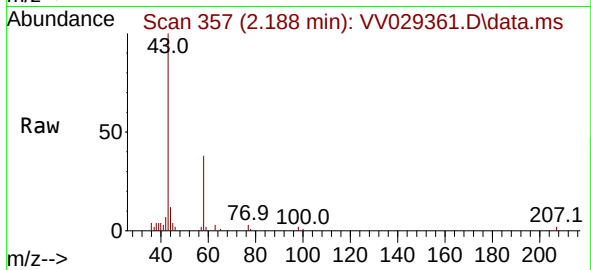

Tgt Ion: 43 Resp: 36171

Ion Ratio Lower Upper

43 100

58 36.0 0.0 70.8

