

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029344.D
 Acq On : 25 Nov 2022 10:13
 Operator : SY/MD
 Sample : N5760-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV2	17990	16657	1.18%	0.202%
2	1.304	76	82	97	rVB	138571	143252	10.11%	1.737%
3	1.564	156	163	175	rVB	98447	111000	7.83%	1.346%
4	2.105	319	331	350	rBV	197569	283424	20.00%	3.436%
5	3.908	881	892	918	rBV2	36304	142004	10.02%	1.722%
6	4.365	1010	1034	1070	rBV3	474477	1416810	100.00%	17.177%
7	5.040	1226	1244	1282	rBV2	329536	839500	59.25%	10.178%
8	5.609	1408	1421	1455	rBV	324516	664897	46.93%	8.061%
9	6.063	1547	1562	1586	rBV2	183344	383693	27.08%	4.652%
10	6.506	1687	1700	1721	rBV2	61508	120061	8.47%	1.456%
11	6.979	1836	1847	1871	rBV	100294	188206	13.28%	2.282%
12	7.310	1937	1950	1965	rBV	435677	767114	54.14%	9.300%
13	7.384	1965	1973	1995	rVB	32225	66898	4.72%	0.811%
14	7.616	2032	2045	2064	rBV	56187	103707	7.32%	1.257%
15	8.088	2178	2192	2232	rBV	272877	664601	46.91%	8.057%
16	8.844	2415	2427	2460	rBV	433819	732054	51.67%	8.875%
17	10.207	2839	2851	2870	rBV	118258	193836	13.68%	2.350%
18	11.239	3160	3172	3195	rBV	475992	750682	52.98%	9.101%
19	11.615	3276	3289	3308	rBV	397970	637473	44.99%	7.728%
20	12.332	3501	3512	3526	rBV5	14387	22652	1.60%	0.275%




Sum of corrected areas: 8248521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029344.D
Acq On : 25 Nov 2022 10:13
Operator : SY/MD
Sample : N5760-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

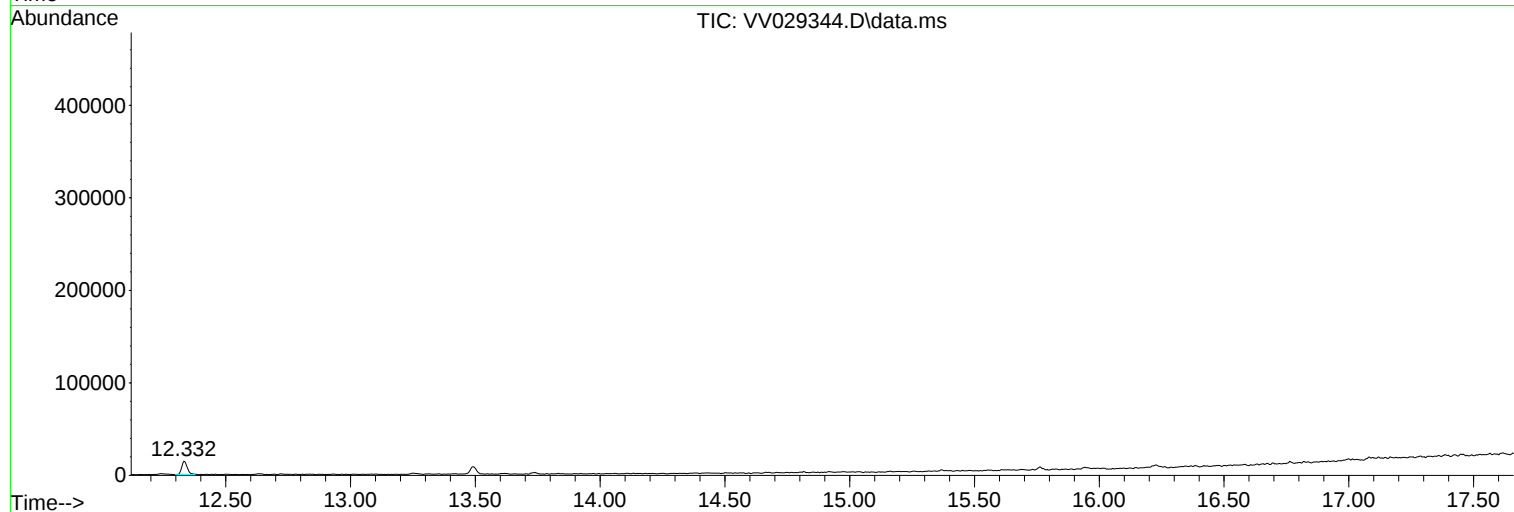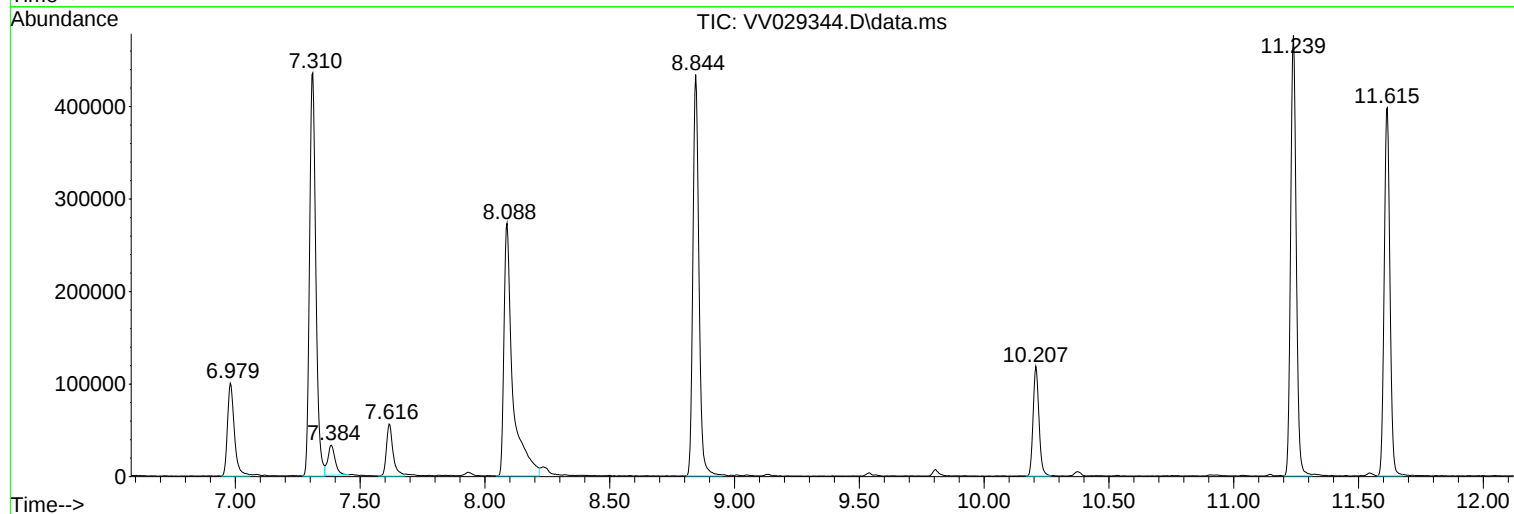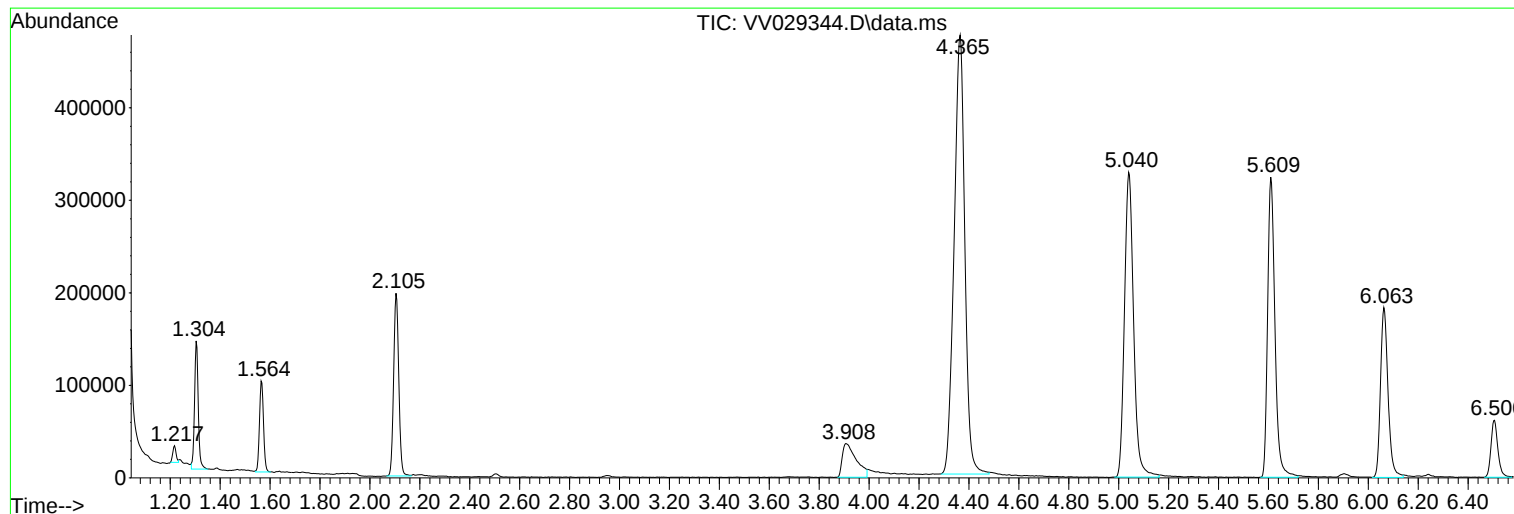

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029344.D
Acq On : 25 Nov 2022 10:13
Operator : SY/MD
Sample : N5760-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029344.D
Acq On : 25 Nov 2022 10:13
Operator : SY/MD
Sample : N5760-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
