

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029349.D
 Acq On : 25 Nov 2022 12:16
 Operator : SY/MD
 Sample : VIBLK233
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK233

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	163559	182682	19.68%	2.282%
2	1.564	156	163	176	rVB	116026	133048	14.33%	1.662%
3	2.105	320	331	347	rBV	222024	319771	34.44%	3.995%
4	3.899	876	889	931	rBV2	67755	300513	32.37%	3.754%
5	4.339	1008	1026	1050	rBV	148843	376540	40.55%	4.704%
6	5.040	1225	1244	1270	rBV2	368701	928495	100.00%	11.599%
7	5.609	1408	1421	1452	rBV	313567	654076	70.44%	8.171%
8	5.902	1500	1512	1524	rBV6	5405	12210	1.32%	0.153%
9	6.063	1546	1562	1595	rBV	205977	437397	47.11%	5.464%
10	6.979	1834	1847	1868	rBV	105772	202066	21.76%	2.524%
11	7.307	1936	1949	1973	rBV	466647	848561	91.39%	10.601%
12	7.616	2033	2045	2069	rBV	58967	109842	11.83%	1.372%
13	8.088	2178	2192	2236	rBV2	349894	823949	88.74%	10.293%
14	8.844	2414	2427	2465	rBV	443741	752657	81.06%	9.403%
15	10.207	2839	2851	2868	rBV	146779	233677	25.17%	2.919%
16	11.239	3159	3172	3192	rBV	483246	753914	81.20%	9.418%
17	11.612	3276	3288	3308	rBV	445898	713953	76.89%	8.919%
18	12.837	3650	3669	3686	rBV3	34081	66687	7.18%	0.833%
19	14.805	4272	4281	4293	rBV2	32130	44955	4.84%	0.562%
20	14.889	4303	4307	4319	rVB10	7632	10912	1.18%	0.136%
21	15.760	4569	4578	4603	rBV2	59926	98955	10.66%	1.236%




Sum of corrected areas: 8004860

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029349.D
Acq On : 25 Nov 2022 12:16
Operator : SY/MD
Sample : VIBLK233
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

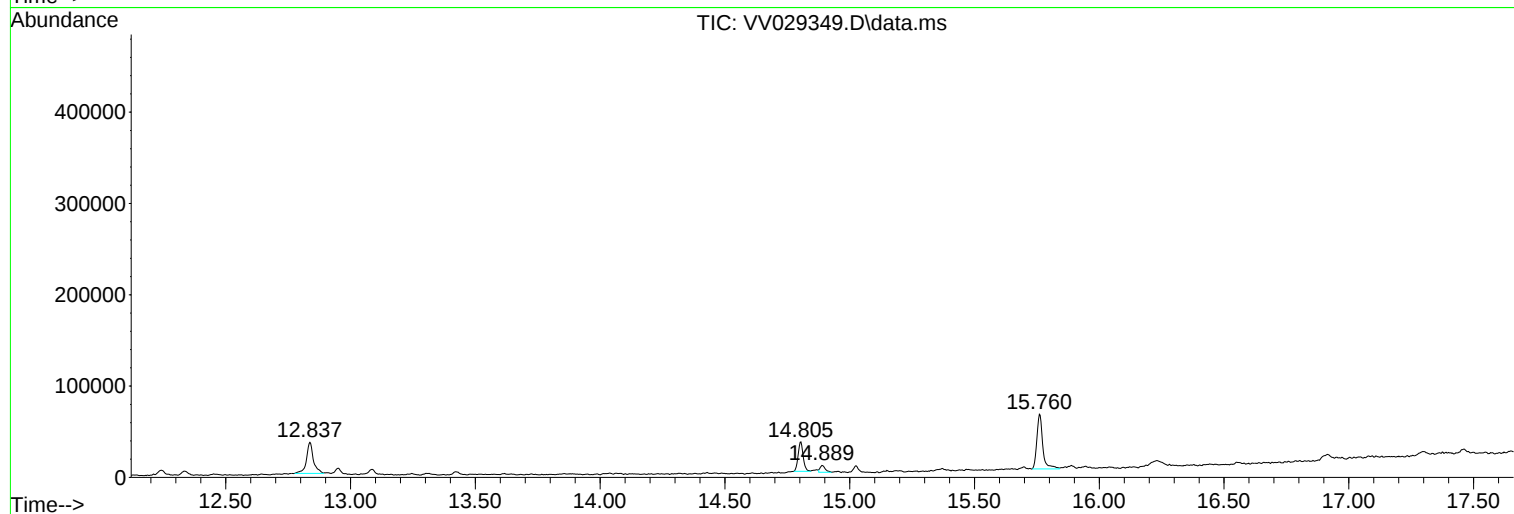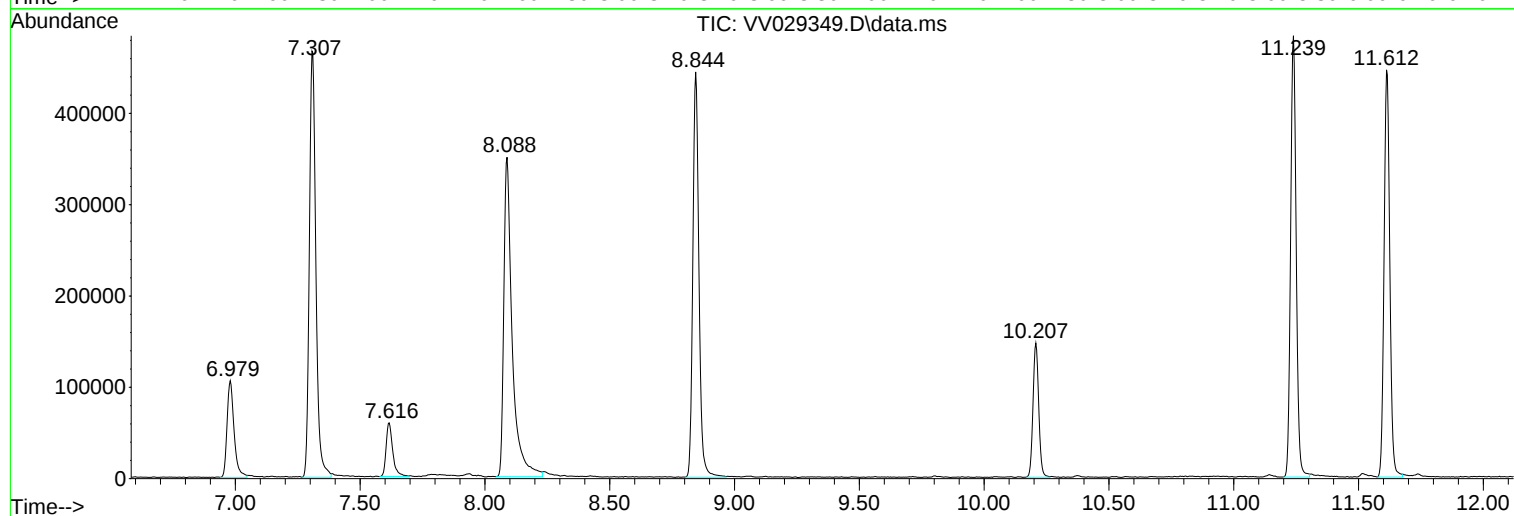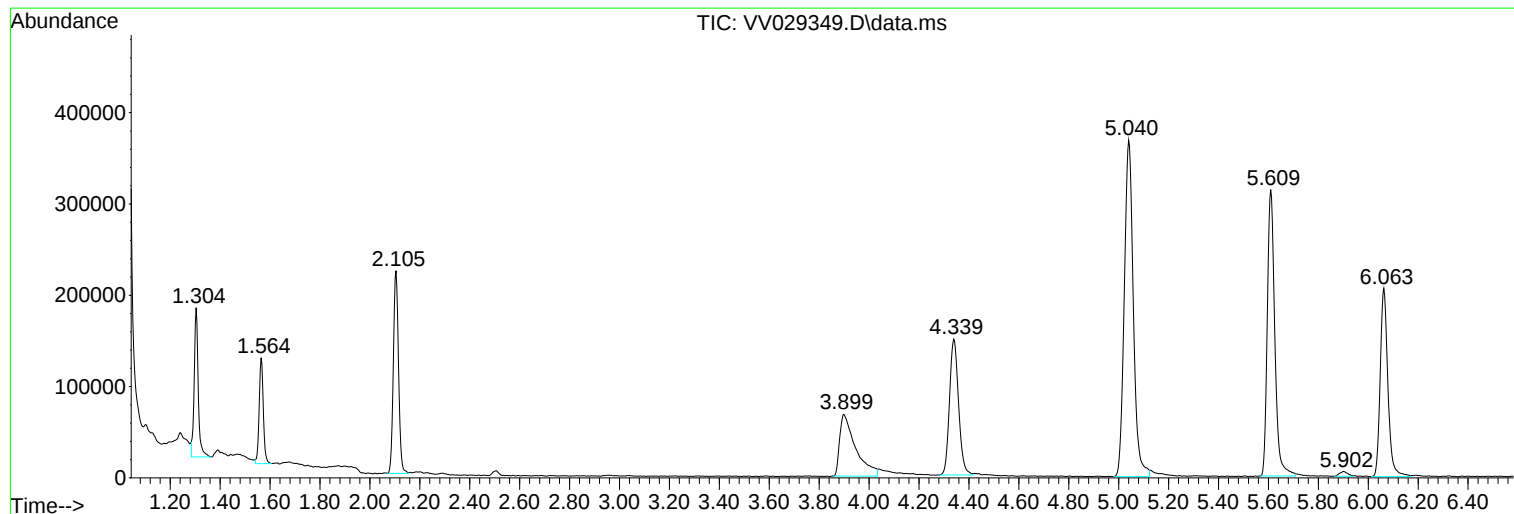

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029349.D
Acq On : 25 Nov 2022 12:16
Operator : SY/MD
Sample : VIBLK233
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK233










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Dodecane, 1-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.760	0.66 ug/L	98955	1,4-Dichlorobenzene-d4	11.239

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	91
2		Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	86
3		1-Chloroundecane	190	C11H23Cl	002473-03-2	86
4		Dodecane, 1-chloro-	204	C12H25Cl	000112-52-7	80
5		Decane, 1-chloro-	176	C10H21Cl	001002-69-3	64

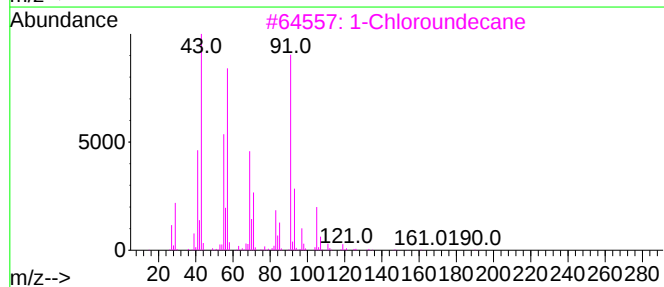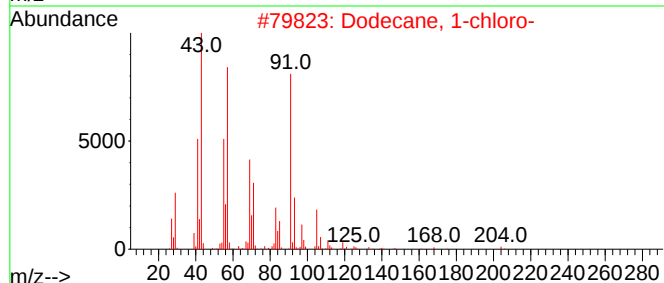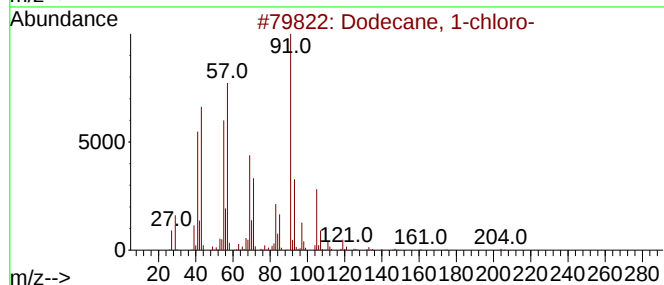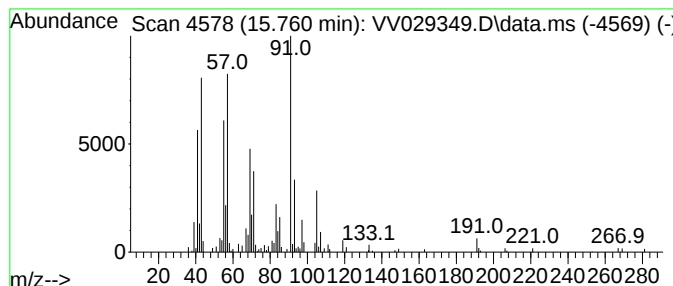

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112522\
Data File : VW029349.D
Acq On : 25 Nov 2022 12:16
Operator : SY/MD
Sample : VIBLK233
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane, 1-chl...	15.760	0.7	ug/L	98955	3	11.239	753914	5.0