

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029358.D
 Acq On : 25 Nov 2022 16:12
 Operator : SY/MD
 Sample : N5770-06DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1G3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	23	27	40	rVB2	24897	30455	3.49%	0.388%
2	1.304	75	82	100	rVB	139256	151521	17.38%	1.929%
3	1.565	155	163	176	rVB	103722	117649	13.49%	1.498%
4	2.102	318	330	346	rBV	196903	285905	32.79%	3.641%
5	2.500	444	454	467	rBV	29358	49526	5.68%	0.631%
6	2.764	521	536	561	rBV2	172165	379344	43.51%	4.830%
7	3.912	877	893	956	rBV2	61518	368279	42.24%	4.689%
8	4.339	1008	1026	1057	rBV2	138076	349215	40.05%	4.447%
9	5.040	1225	1244	1289	rBV2	343164	871888	100.00%	11.102%
10	5.609	1408	1421	1454	rBV	292341	606700	69.58%	7.725%
11	5.908	1499	1514	1530	rBV6	7550	16571	1.90%	0.211%
12	6.063	1547	1562	1591	rBV	188490	395408	45.35%	5.035%
13	6.979	1836	1847	1877	rBV	99311	193757	22.22%	2.467%
14	7.307	1935	1949	1988	rBV	441151	785350	90.07%	10.000%
15	7.616	2034	2045	2071	rBV	57359	107266	12.30%	1.366%
16	8.088	2178	2192	2233	rBV2	364257	776625	89.07%	9.889%
17	8.844	2413	2427	2448	rBV	414429	691015	79.26%	8.799%
18	10.207	2838	2851	2865	rBV	139318	217950	25.00%	2.775%
19	11.239	3157	3172	3188	rBV	438889	691875	79.35%	8.810%
20	11.545	3253	3267	3275	rBV5	5668	9927	1.14%	0.126%
21	11.612	3276	3288	3313	rVV	426595	676504	77.59%	8.614%
22	12.837	3662	3669	3685	rVB8	4527	8801	1.01%	0.112%
23	13.612	3898	3910	3918	rBV3	5104	9137	1.05%	0.116%
24	14.805	4273	4281	4291	rVB2	8493	12173	1.40%	0.155%
25	15.368	4445	4456	4463	rBV8	8072	14074	1.61%	0.179%
26	15.760	4570	4578	4597	rBV3	22067	36395	4.17%	0.463%




Sum of corrected areas: 7853310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029358.D
Acq On : 25 Nov 2022 16:12
Operator : SY/MD
Sample : N5770-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

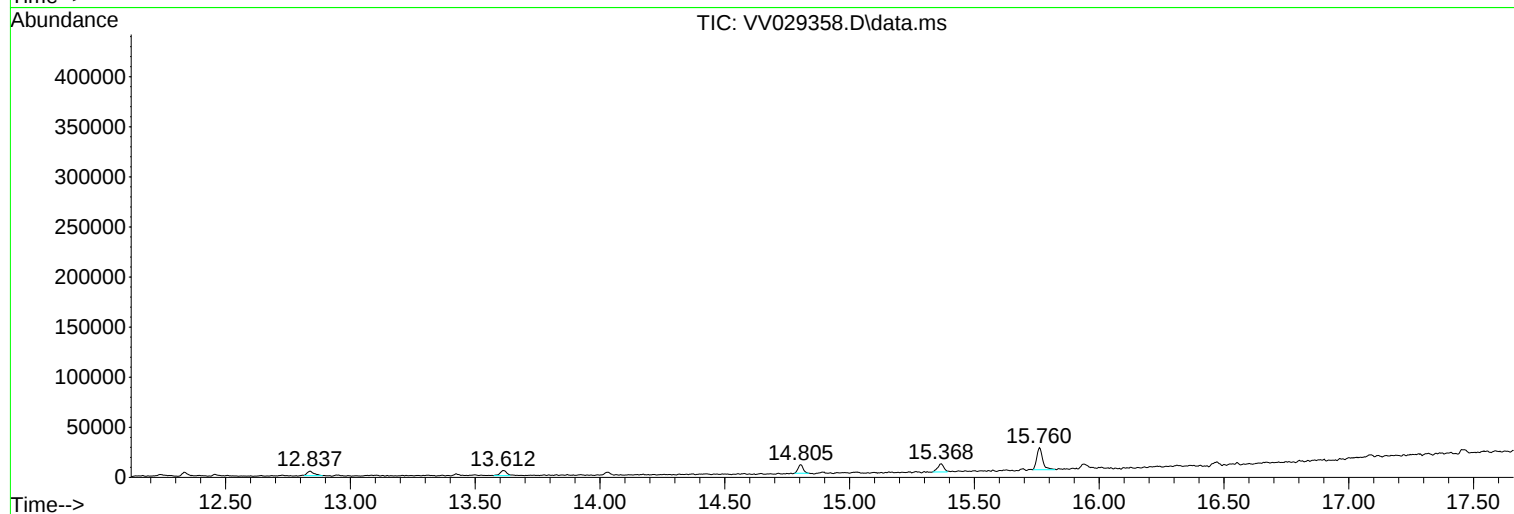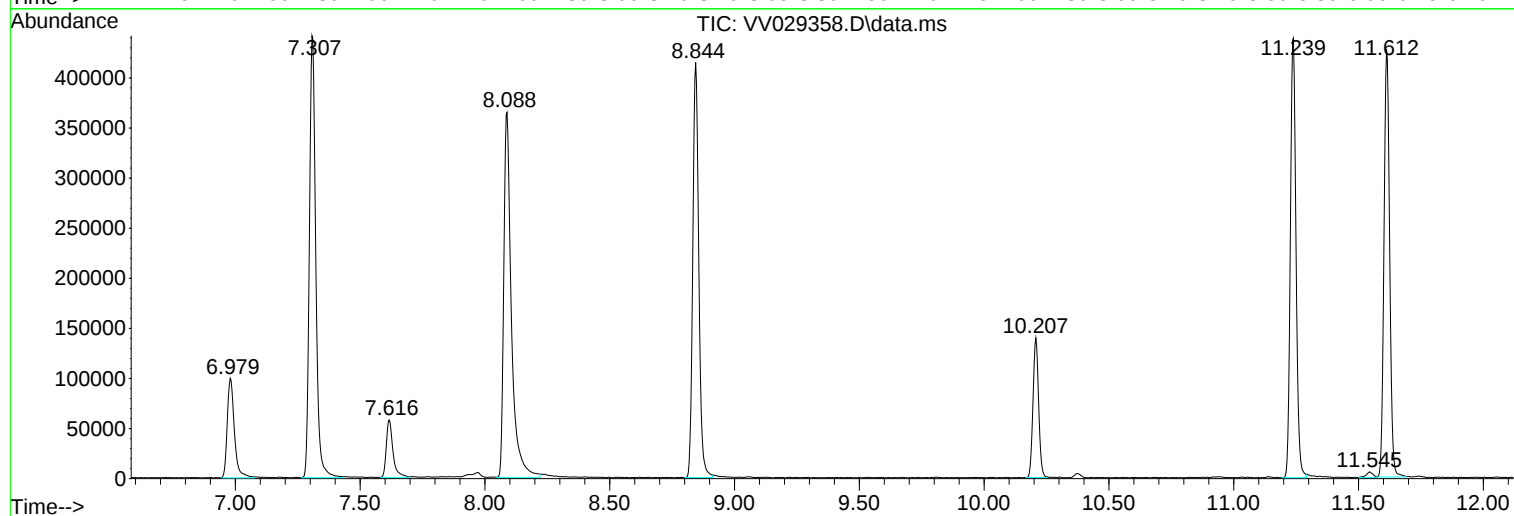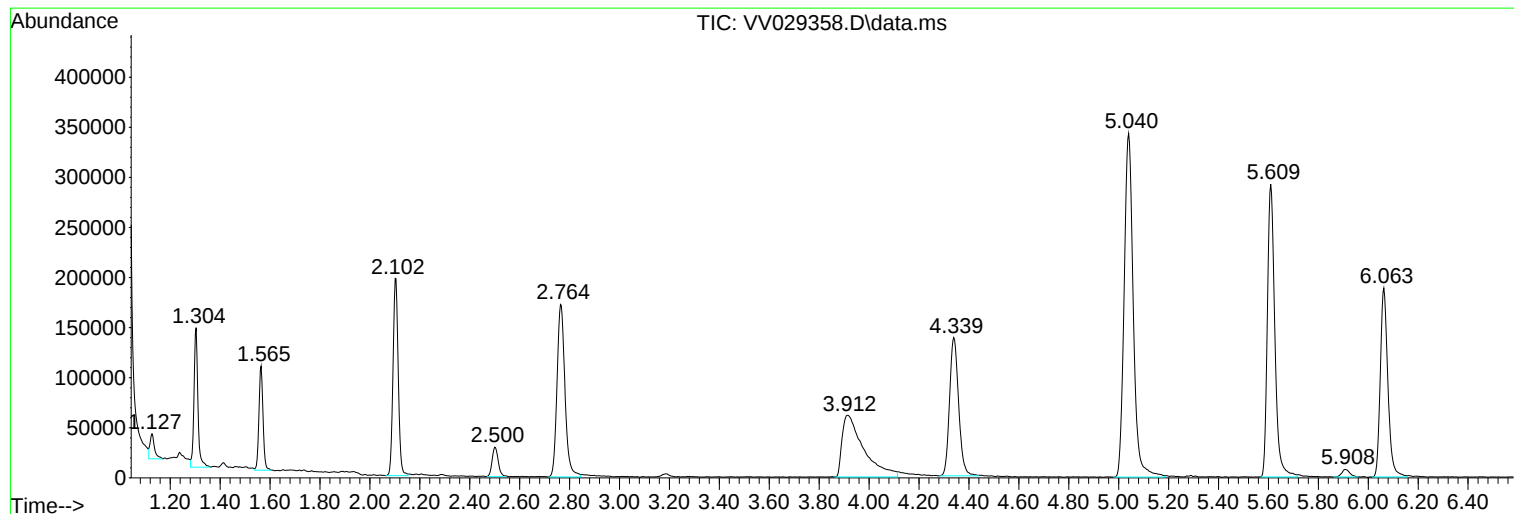

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029358.D
Acq On : 25 Nov 2022 16:12
Operator : SY/MD
Sample : N5770-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029358.D
Acq On : 25 Nov 2022 16:12
Operator : SY/MD
Sample : N5770-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc