

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029359.D
 Acq On : 25 Nov 2022 16:36
 Operator : SY/MD
 Sample : N5770-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	58	62	75	rVV	13880	17812	2.03%	0.233%
2	1.304	76	82	101	rVB	142240	149369	17.02%	1.952%
3	1.564	156	163	175	rVB	103018	115785	13.19%	1.513%
4	2.105	320	331	344	rBV	201057	291578	33.22%	3.811%
5	2.182	344	355	383	rVB	19730	58485	6.66%	0.764%
6	3.889	871	886	922	rBV	78607	293217	33.41%	3.832%
7	4.339	1009	1026	1053	rBV	144002	365541	41.65%	4.777%
8	5.040	1224	1244	1271	rBV2	344502	877697	100.00%	11.471%
9	5.609	1407	1421	1463	rBV	313553	653768	74.49%	8.544%
10	5.908	1503	1514	1532	rVB8	12296	27742	3.16%	0.363%
11	6.063	1546	1562	1588	rBV	193636	408752	46.57%	5.342%
12	6.979	1834	1847	1874	rBV	102611	194396	22.15%	2.541%
13	7.310	1935	1950	1984	rBV	437935	798356	90.96%	10.434%
14	7.616	2035	2045	2070	rBV	58570	105992	12.08%	1.385%
15	7.969	2147	2155	2167	rVB4	11808	20859	2.38%	0.273%
16	8.085	2180	2191	2232	rBV2	384530	787671	89.74%	10.294%
17	8.844	2415	2427	2459	rBV	445403	741868	84.52%	9.695%
18	10.207	2839	2851	2867	rBV	140180	220914	25.17%	2.887%
19	10.374	2893	2903	2917	rVB3	7932	13331	1.52%	0.174%
20	11.239	3155	3172	3192	rBV	468620	728634	83.02%	9.522%
21	11.541	3256	3266	3277	rBV2	20065	35305	4.02%	0.461%
22	11.612	3277	3288	3306	rVV	415989	663485	75.59%	8.671%
23	12.336	3504	3513	3523	rBV2	19107	29209	3.33%	0.382%
24	14.802	4274	4280	4292	rVB9	6326	9342	1.06%	0.122%
25	15.368	4444	4456	4462	rBV9	7036	12513	1.43%	0.164%
26	15.760	4571	4578	4592	rVB3	19801	30130	3.43%	0.394%




Sum of corrected areas: 7651751

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029359.D
Acq On : 25 Nov 2022 16:36
Operator : SY/MD
Sample : N5770-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

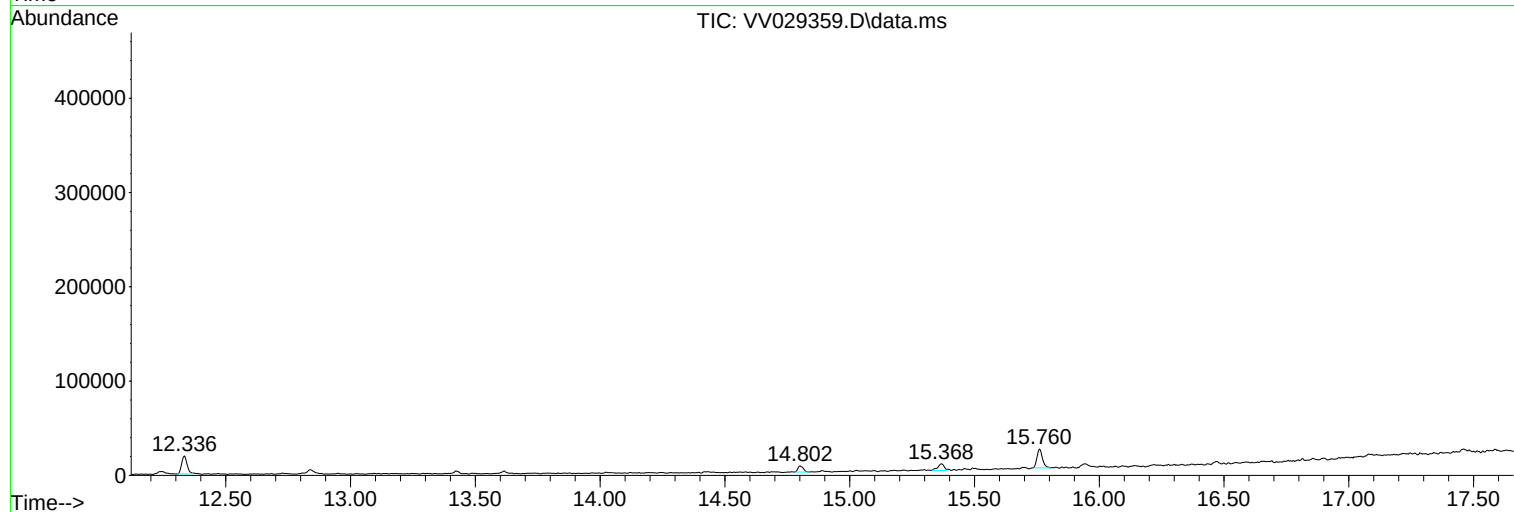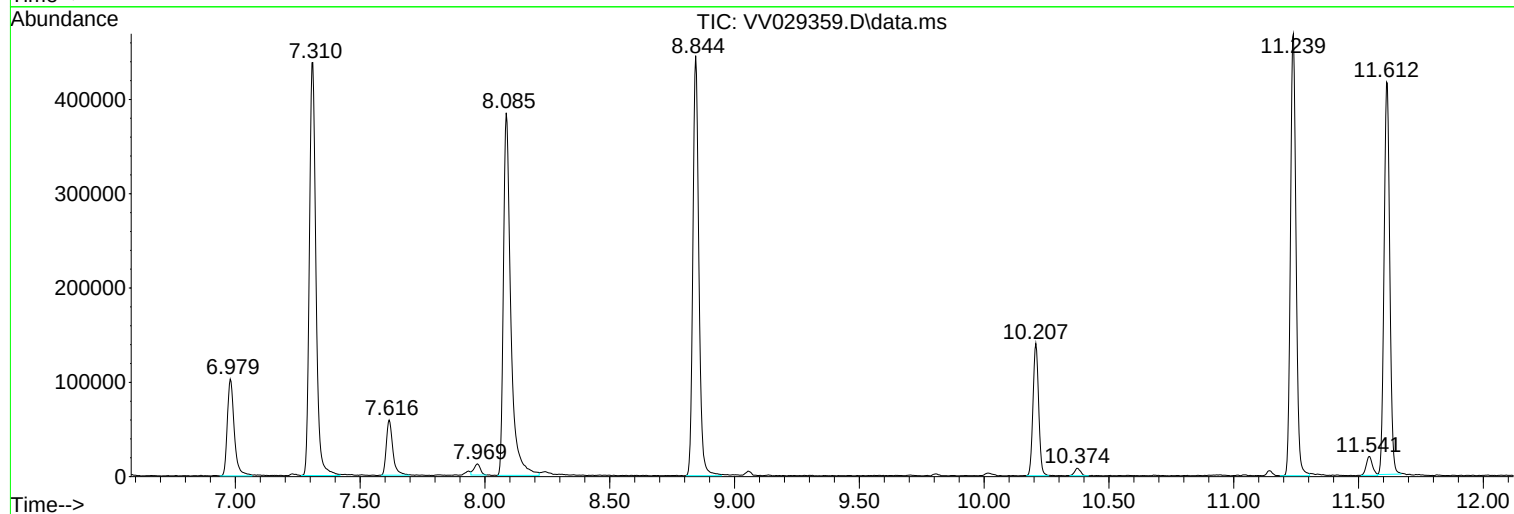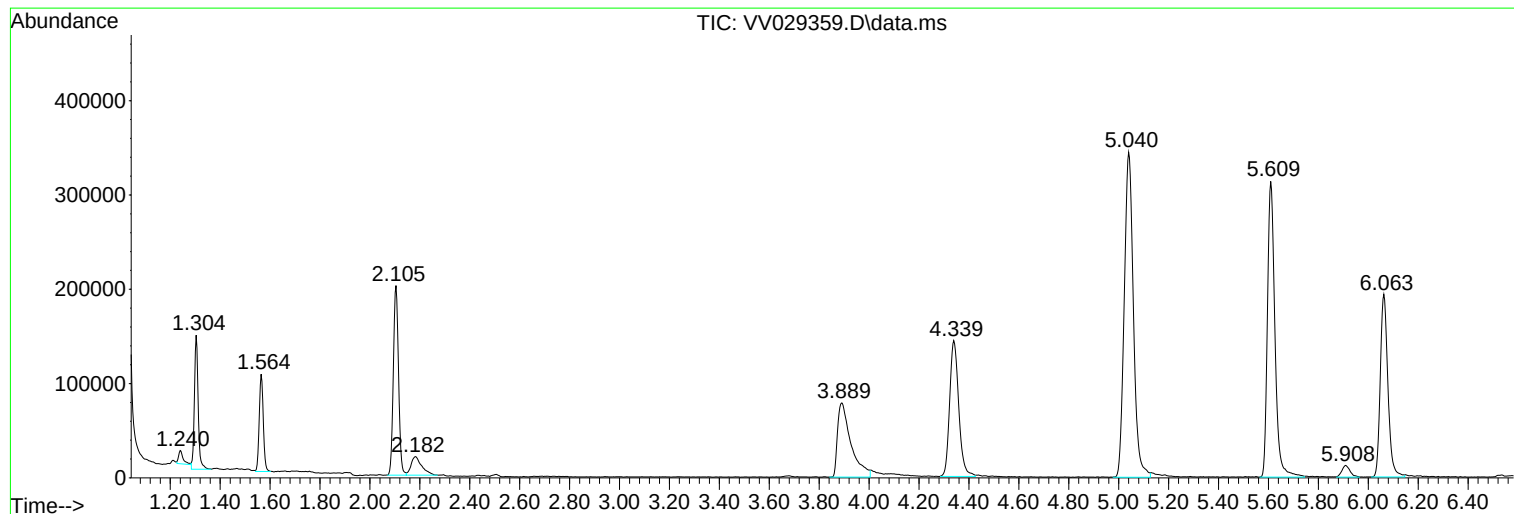

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029359.D
Acq On : 25 Nov 2022 16:36
Operator : SY/MD
Sample : N5770-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029359.D
Acq On : 25 Nov 2022 16:36
Operator : SY/MD
Sample : N5770-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc