

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029360.D
 Acq On : 25 Nov 2022 17:01
 Operator : SY/MD
 Sample : N5770-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1N0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	58	62	74	rVV	17594	20757	2.46%	0.279%
2	1.304	76	82	104	rVB	144990	149266	17.70%	2.003%
3	1.564	156	163	179	rVB	107488	121866	14.45%	1.635%
4	2.105	320	331	344	rBV	192724	278944	33.07%	3.743%
5	2.185	345	356	379	rVB2	17380	49876	5.91%	0.669%
6	3.892	874	887	936	rBV	73790	289538	34.33%	3.885%
7	4.339	1009	1026	1051	rBV2	134955	347942	41.25%	4.668%
8	5.040	1226	1244	1278	rBV2	332683	843465	100.00%	11.317%
9	5.609	1408	1421	1449	rBV	308723	631106	74.82%	8.468%
10	5.908	1501	1514	1534	rBV6	11610	26317	3.12%	0.353%
11	6.063	1547	1562	1586	rBV	184061	388622	46.07%	5.214%
12	6.979	1836	1847	1871	rBV	98204	184120	21.83%	2.470%
13	7.307	1935	1949	1970	rBV	425718	761781	90.32%	10.221%
14	7.616	2030	2045	2073	rBV	56777	105674	12.53%	1.418%
15	7.969	2147	2155	2166	rVB3	11595	21206	2.51%	0.285%
16	8.085	2179	2191	2232	rBV2	372475	761081	90.23%	10.212%
17	8.844	2414	2427	2456	rBV	427847	722348	85.64%	9.692%
18	10.207	2838	2851	2867	rBV	132616	210832	25.00%	2.829%
19	10.374	2892	2903	2917	rVB3	9165	15408	1.83%	0.207%
20	11.239	3160	3172	3199	rBV	473567	743365	88.13%	9.974%
21	11.542	3254	3266	3277	rBV2	21532	40714	4.83%	0.546%
22	11.612	3277	3288	3310	rVB	421066	664314	78.76%	8.913%
23	12.239	3471	3483	3498	rBV5	4105	9156	1.09%	0.123%
24	12.333	3504	3512	3522	rBV2	18801	27606	3.27%	0.370%
25	15.368	4447	4456	4467	rBV2	4958	8958	1.06%	0.120%
26	15.760	4571	4578	4588	rBV3	19778	28742	3.41%	0.386%




Sum of corrected areas: 7453004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029360.D
Acq On : 25 Nov 2022 17:01
Operator : SY/MD
Sample : N5770-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

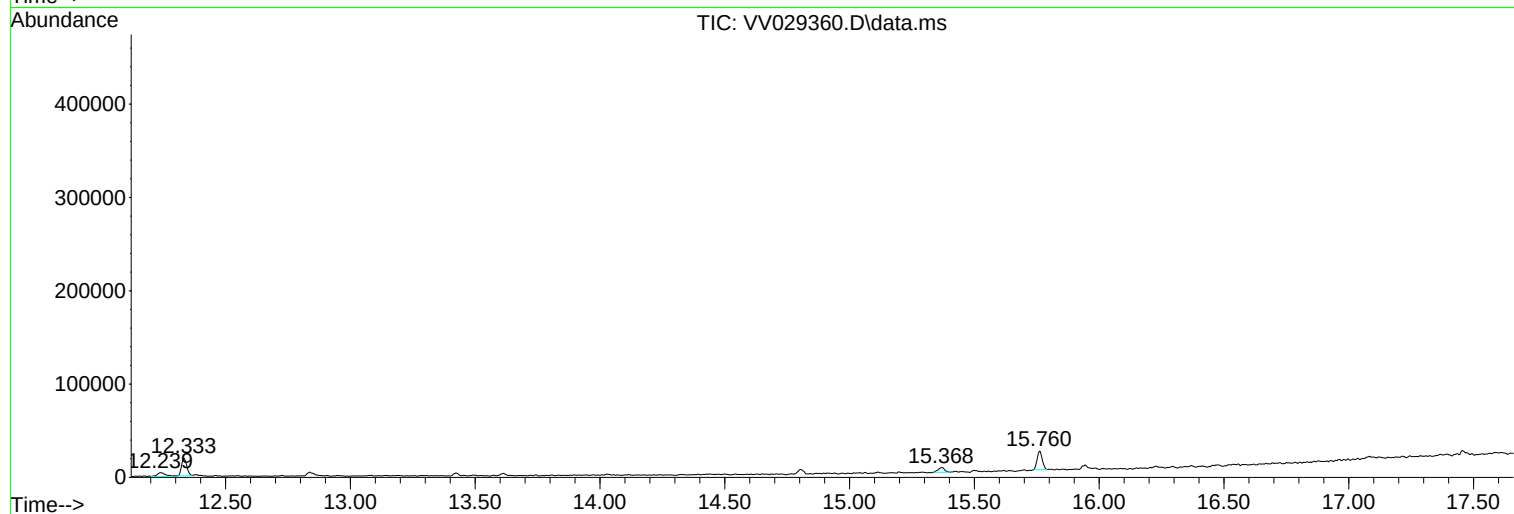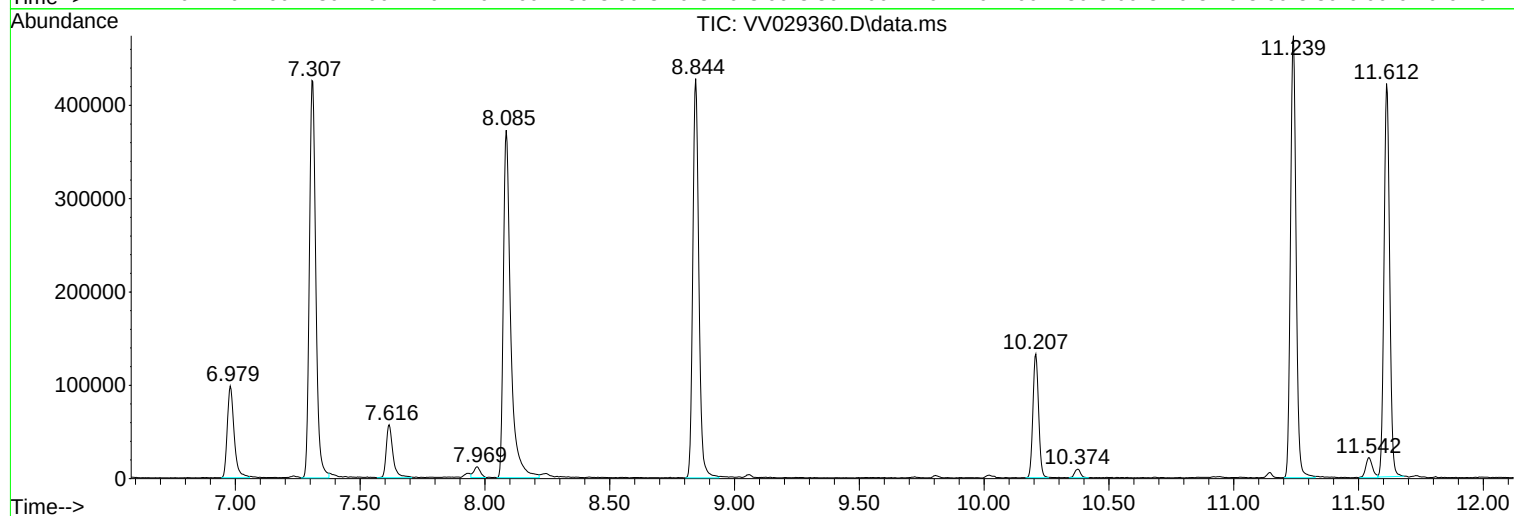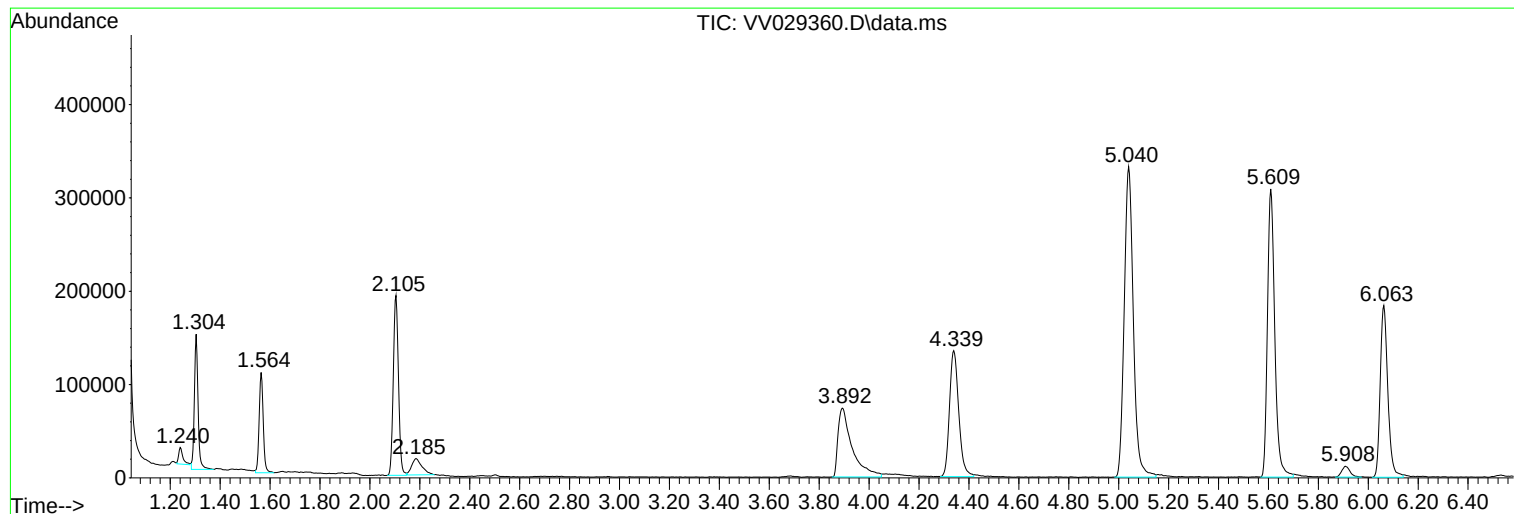

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029360.D
Acq On : 25 Nov 2022 17:01
Operator : SY/MD
Sample : N5770-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029360.D
Acq On : 25 Nov 2022 17:01
Operator : SY/MD
Sample : N5770-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc