

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029362.D
 Acq On : 25 Nov 2022 17:50
 Operator : SY/MD
 Sample : N5770-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	152441	156248	16.59%	1.996%
2	1.564	155	163	174	rVB	111750	124867	13.26%	1.595%
3	2.105	320	331	348	rBV	214505	308237	32.73%	3.937%
4	3.905	875	891	939	rBV3	62344	298565	31.70%	3.814%
5	4.339	1007	1026	1052	rBV	149509	375856	39.91%	4.801%
6	5.040	1227	1244	1282	rBV2	367263	941838	100.00%	12.031%
7	5.609	1408	1421	1450	rBV	324415	664941	70.60%	8.494%
8	6.063	1545	1562	1590	rBV	204284	426426	45.28%	5.447%
9	6.979	1835	1847	1877	rBV	109065	209777	22.27%	2.680%
10	7.307	1937	1949	1973	rBV	470708	845022	89.72%	10.794%
11	7.616	2033	2045	2064	rBV	62215	113888	12.09%	1.455%
12	8.085	2178	2191	2240	rBV	384005	818572	86.91%	10.457%
13	8.844	2412	2427	2454	rBV	453032	767711	81.51%	9.807%
14	10.207	2836	2851	2867	rBV	150572	236181	25.08%	3.017%
15	10.378	2892	2904	2914	rBV3	5279	10169	1.08%	0.130%
16	11.239	3156	3172	3192	rBV	487882	768918	81.64%	9.822%
17	11.542	3254	3266	3277	rBV4	15582	28866	3.06%	0.369%
18	11.612	3277	3288	3311	rVB	444059	702606	74.60%	8.975%
19	15.760	4570	4578	4590	rVB3	18970	29619	3.14%	0.378%




Sum of corrected areas: 7828307

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029362.D
Acq On : 25 Nov 2022 17:50
Operator : SY/MD
Sample : N5770-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

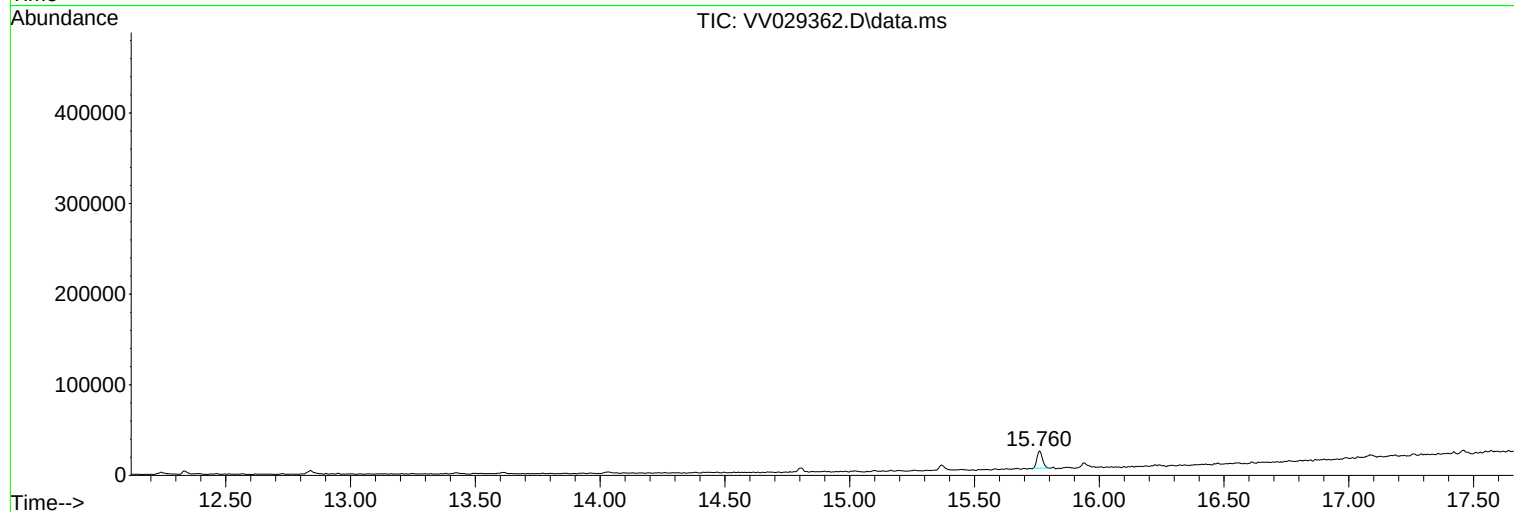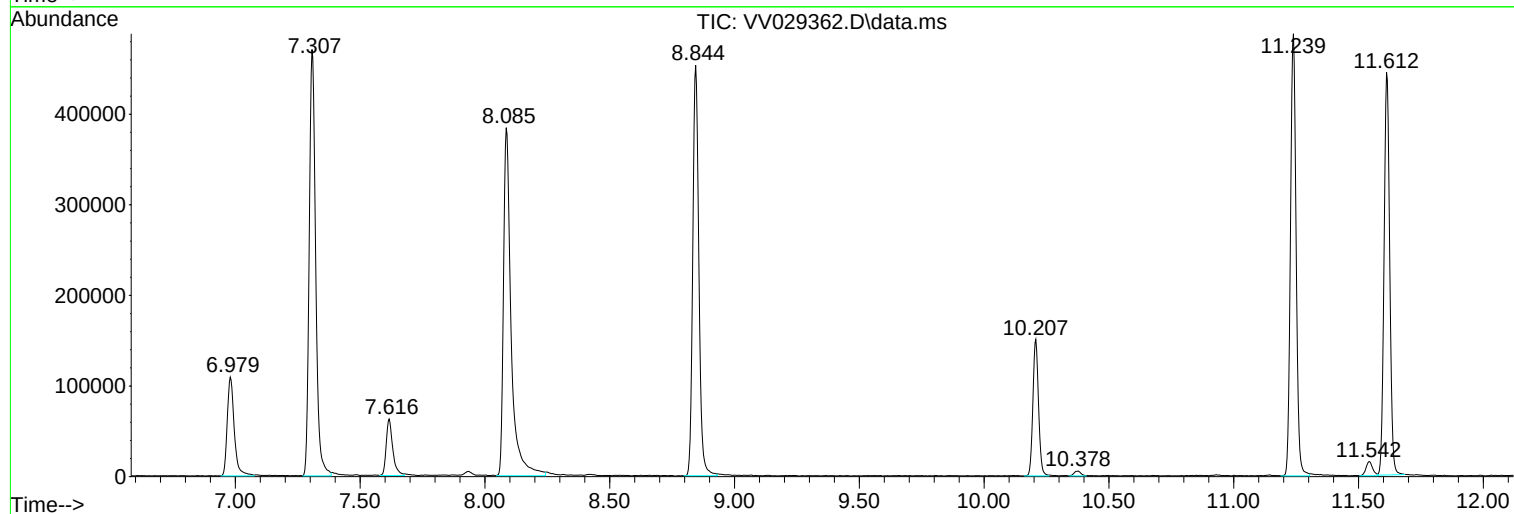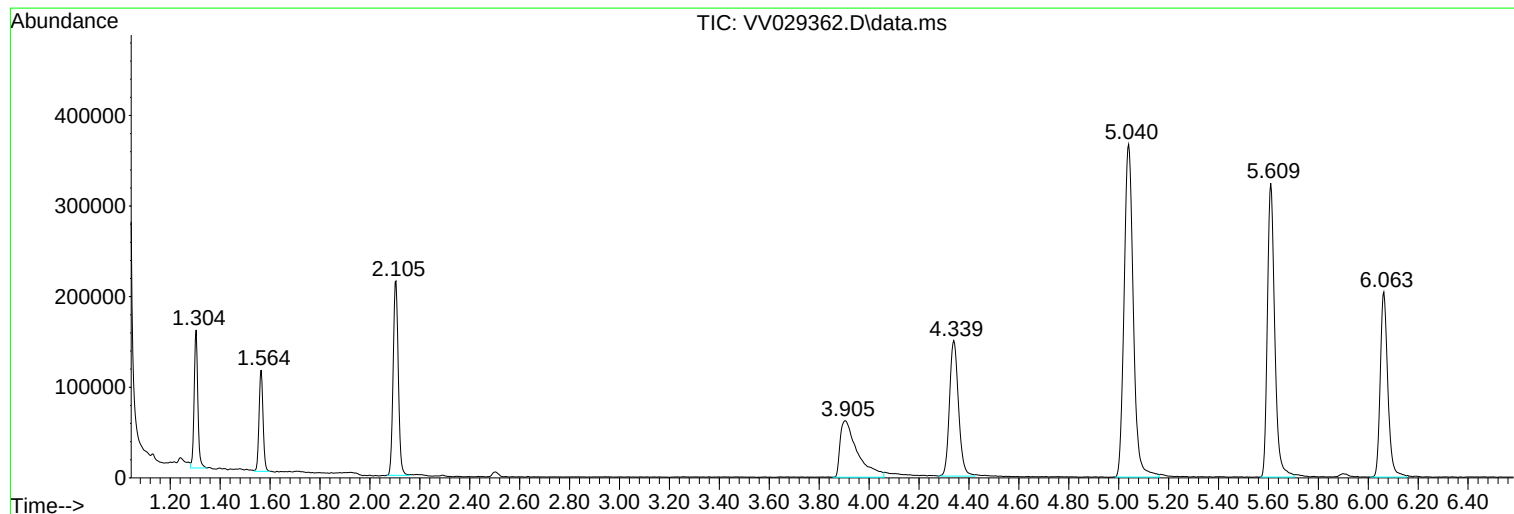

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029362.D
Acq On : 25 Nov 2022 17:50
Operator : SY/MD
Sample : N5770-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029362.D
Acq On : 25 Nov 2022 17:50
Operator : SY/MD
Sample : N5770-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc