

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029363.D
 Acq On : 25 Nov 2022 18:40
 Operator : SY/MD
 Sample : N5759-01DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB76DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV	30730	26544	3.11%	0.304%
2	1.304	75	82	103	rVB2	163260	180073	21.09%	2.064%
3	1.564	156	163	176	rVB	99906	114606	13.42%	1.313%
4	2.104	320	331	351	rBV3	226140	362229	42.43%	4.151%
5	2.500	445	454	468	rBV	30605	51458	6.03%	0.590%
6	3.182	650	666	681	rBV	62542	133704	15.66%	1.532%
7	3.905	873	891	949	rBV3	250139	845329	99.01%	9.688%
8	4.339	1008	1026	1049	rBV	138420	344691	40.37%	3.950%
9	4.600	1088	1107	1128	rBV3	99259	248963	29.16%	2.853%
10	5.040	1227	1244	1267	rBV2	339982	853779	100.00%	9.785%
11	5.609	1406	1421	1450	rBV	301769	622286	72.89%	7.132%
12	5.908	1501	1514	1532	rBV	118513	242445	28.40%	2.779%
13	6.063	1548	1562	1596	rBV	187284	392933	46.02%	4.503%
14	6.979	1836	1847	1874	rBV	97865	191125	22.39%	2.190%
15	7.307	1937	1949	1986	rBV	429448	778378	91.17%	8.921%
16	7.616	2035	2045	2065	rBV	54572	102008	11.95%	1.169%
17	7.934	2134	2144	2152	rBV	5945	10095	1.18%	0.116%
18	8.088	2180	2192	2227	rBV2	369317	772154	90.44%	8.849%
19	8.844	2413	2427	2450	rBV	429950	715084	83.76%	8.195%
20	10.207	2837	2851	2865	rBV	141545	222409	26.05%	2.549%
21	10.374	2893	2903	2916	rBV2	9734	15925	1.87%	0.183%
22	11.239	3160	3172	3193	rBV	459915	724250	84.83%	8.300%
23	11.612	3276	3288	3311	rBV	407233	656929	76.94%	7.529%
24	13.249	3789	3797	3809	rVB3	6914	11315	1.33%	0.130%
25	13.493	3856	3873	3886	rVB	22389	49170	5.76%	0.564%
26	13.734	3937	3948	3956	rBV2	8100	13802	1.62%	0.158%
27	15.368	4450	4456	4467	rVB2	6047	9265	1.09%	0.106%
28	15.763	4571	4579	4588	rBV4	16286	24235	2.84%	0.278%
29	15.940	4628	4634	4646	rBV4	5510	10470	1.23%	0.120%




Sum of corrected areas: 8725654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029363.D
Acq On : 25 Nov 2022 18:40
Operator : SY/MD
Sample : N5759-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

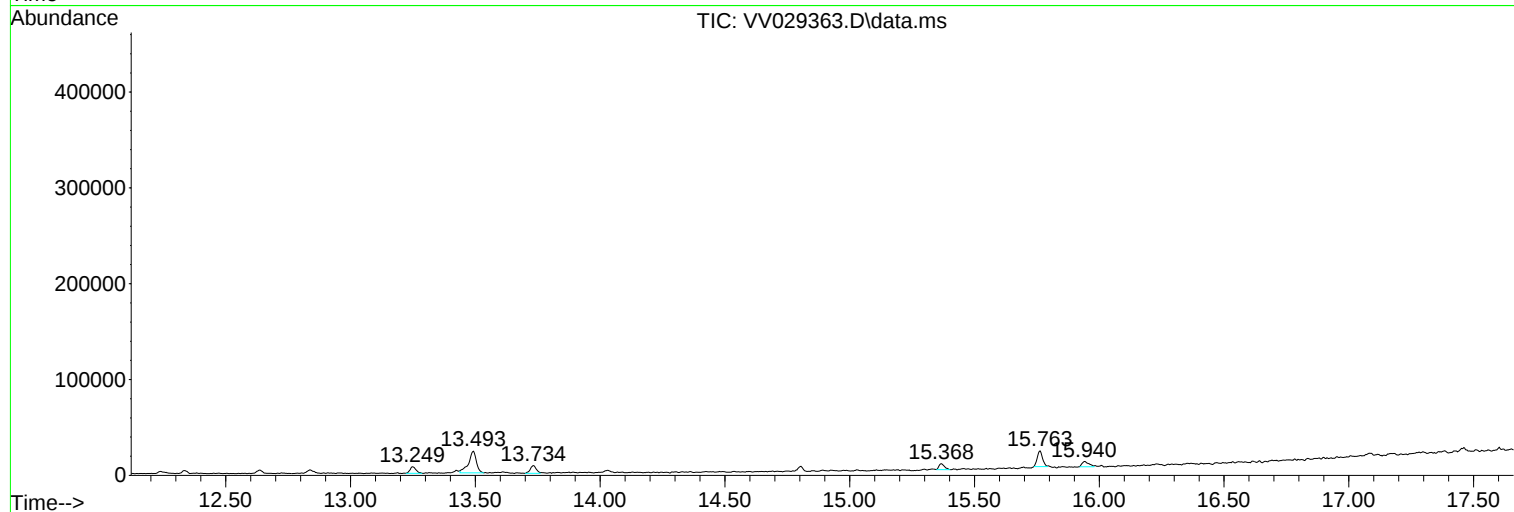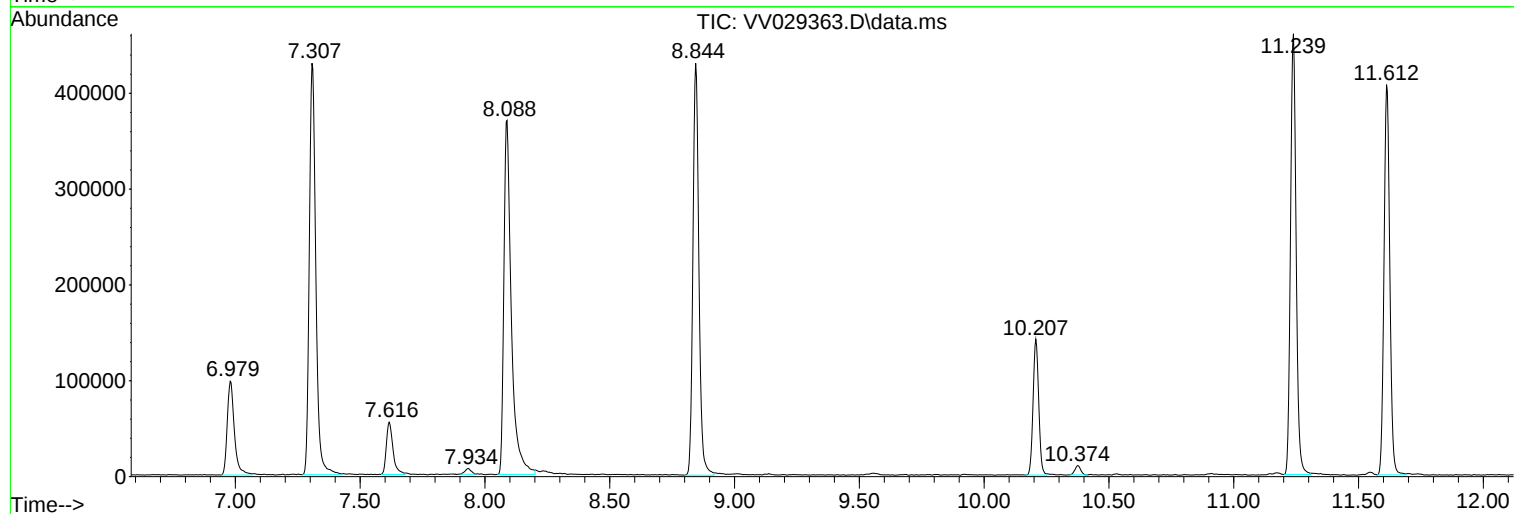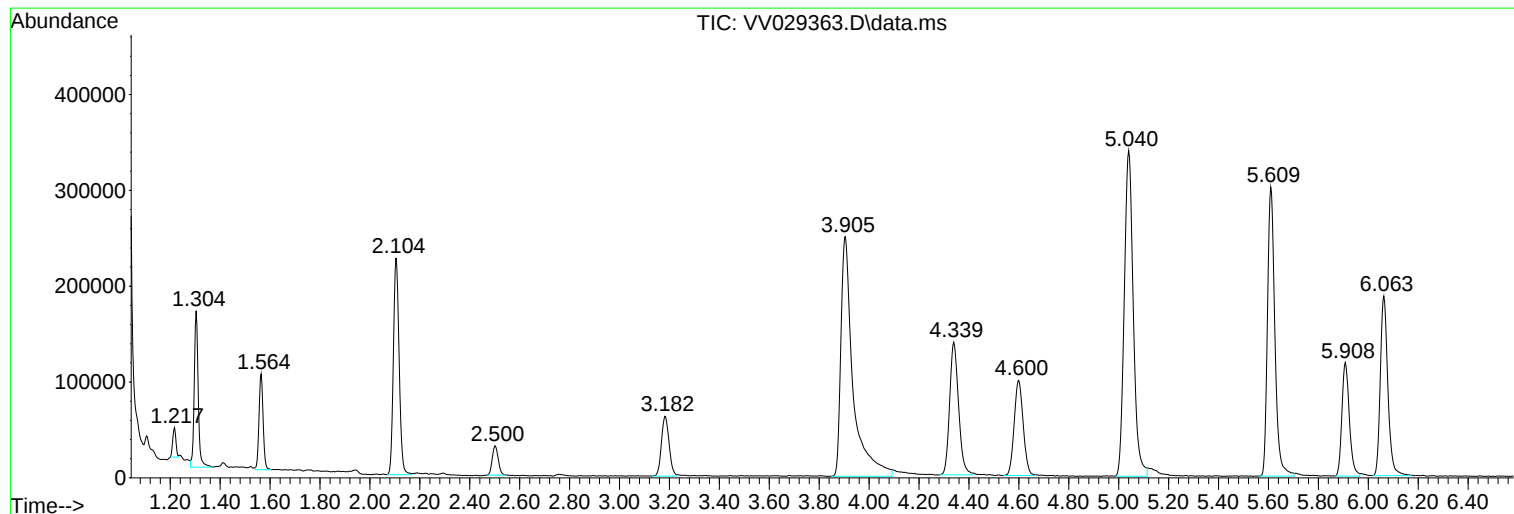

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029363.D
Acq On : 25 Nov 2022 18:40
Operator : SY/MD
Sample : N5759-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029363.D
Acq On : 25 Nov 2022 18:40
Operator : SY/MD
Sample : N5759-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc