

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029364.D
 Acq On : 25 Nov 2022 19:02
 Operator : SY/MD
 Sample : N5770-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB78

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	132256	134306	16.20%	1.858%
2	1.564	156	163	174	rVB	98607	107418	12.96%	1.486%
3	2.105	320	331	347	rBV	190934	273660	33.01%	3.787%
4	3.921	881	896	958	rBV2	48329	285341	34.42%	3.948%
5	4.342	1010	1027	1055	rBV	133982	333207	40.20%	4.611%
6	5.043	1227	1245	1270	rBV2	329042	828946	100.00%	11.470%
7	5.612	1407	1422	1453	rBV	308647	632183	76.26%	8.747%
8	6.066	1549	1563	1593	rBV	180953	385906	46.55%	5.340%
9	6.982	1834	1848	1878	rBV	96381	185991	22.44%	2.574%
10	7.310	1936	1950	1991	rBV	423918	759845	91.66%	10.514%
11	7.619	2035	2046	2073	rBV	54131	101923	12.30%	1.410%
12	7.937	2132	2145	2162	rVB2	11369	22283	2.69%	0.308%
13	8.088	2180	2192	2234	rBV	360638	759839	91.66%	10.514%
14	8.844	2415	2427	2452	rBV	432120	725900	87.57%	10.044%
15	10.207	2839	2851	2865	rBV	134576	213897	25.80%	2.960%
16	10.374	2889	2903	2913	rBV2	19448	32640	3.94%	0.452%
17	11.239	3160	3172	3193	rBV	469214	740149	89.29%	10.241%
18	11.615	3277	3289	3312	rVV	415399	655609	79.09%	9.072%
19	12.239	3470	3483	3495	rBV3	6124	10931	1.32%	0.151%
20	13.493	3861	3873	3883	rBV2	6351	10543	1.27%	0.146%
21	15.760	4570	4578	4588	rBV3	16839	26586	3.21%	0.368%




Sum of corrected areas: 7227103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029364.D
Acq On : 25 Nov 2022 19:02
Operator : SY/MD
Sample : N5770-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

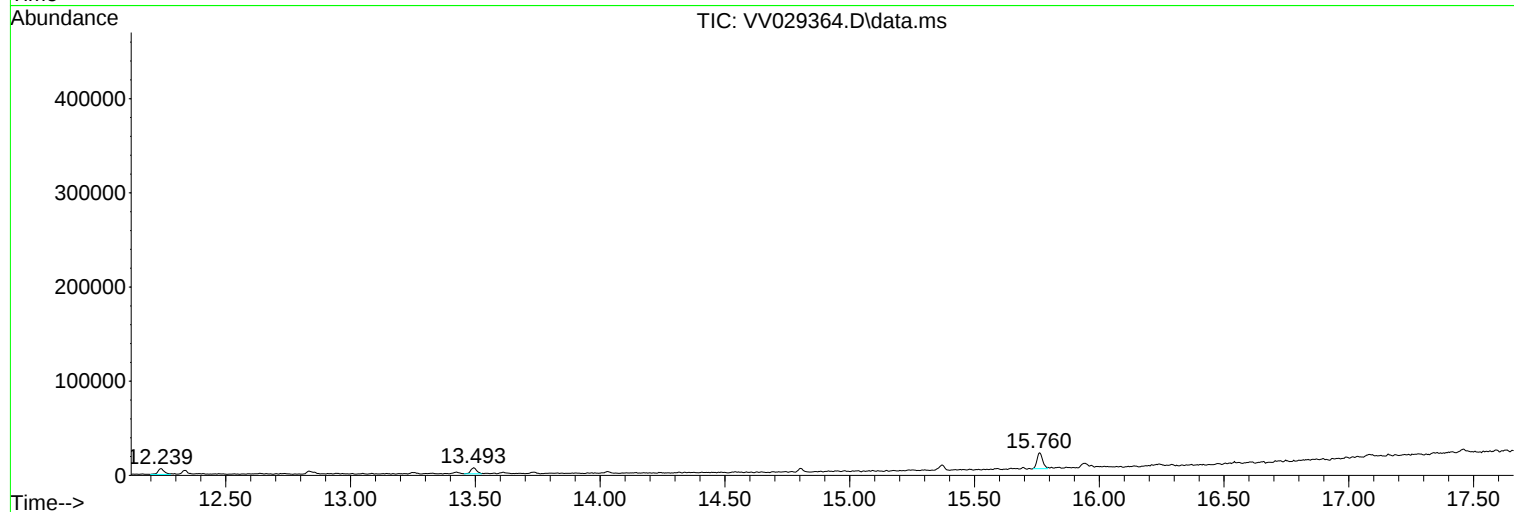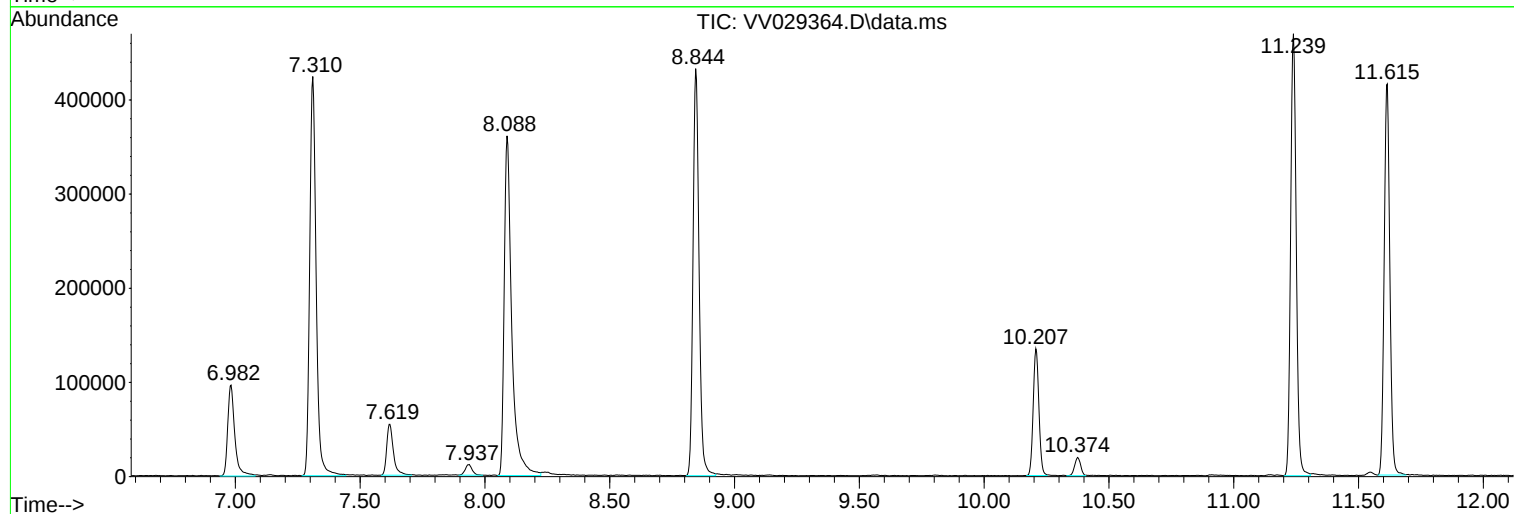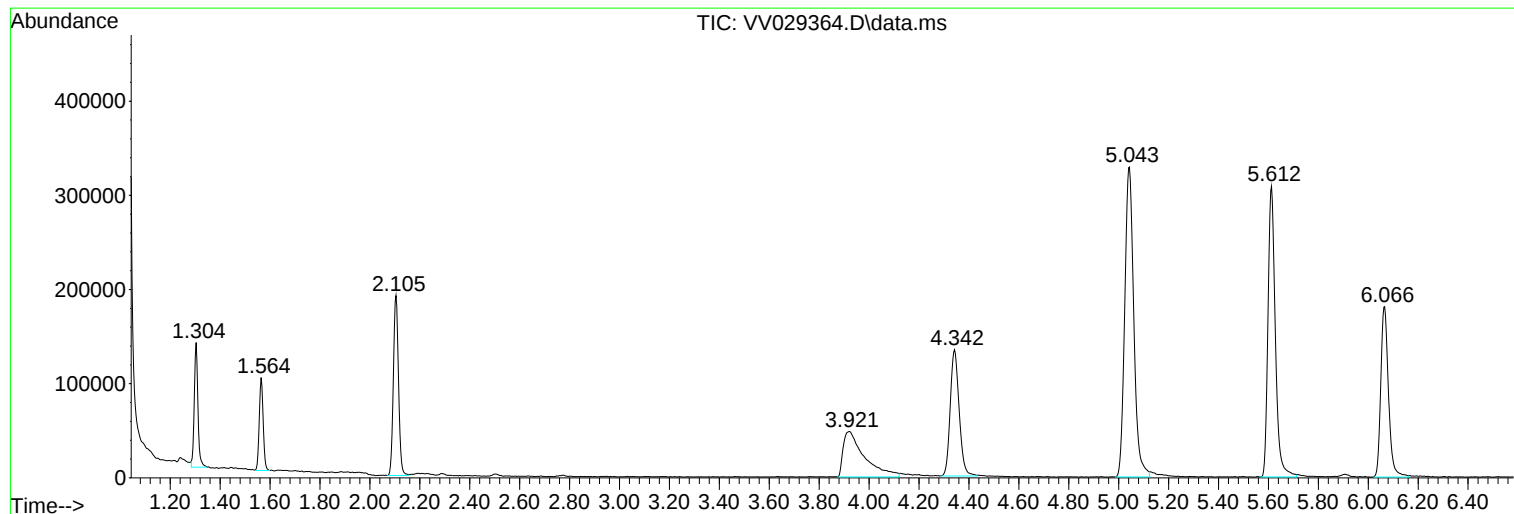

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029364.D
Acq On : 25 Nov 2022 19:02
Operator : SY/MD
Sample : N5770-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029364.D
Acq On : 25 Nov 2022 19:02
Operator : SY/MD
Sample : N5770-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc