

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029365.D
 Acq On : 25 Nov 2022 19:27
 Operator : SY/MD
 Sample : N5770-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB79

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	136494	149088	17.11%	1.985%
2	1.564	155	163	179	rVB	101469	117038	13.43%	1.558%
3	2.101	319	330	344	rBV	195749	283698	32.55%	3.777%
4	3.908	879	892	944	rBV2	53864	289565	33.23%	3.855%
5	4.339	1009	1026	1054	rBV	137496	350606	40.23%	4.668%
6	5.040	1226	1244	1277	rBV2	343940	871526	100.00%	11.603%
7	5.609	1407	1421	1455	rBV	318747	651934	74.80%	8.680%
8	6.063	1547	1562	1598	rBV	191115	401859	46.11%	5.350%
9	6.979	1834	1847	1878	rBV2	99048	190815	21.89%	2.541%
10	7.307	1937	1949	1975	rBV	435580	787300	90.34%	10.482%
11	7.616	2033	2045	2064	rBV2	57772	105765	12.14%	1.408%
12	7.934	2133	2144	2157	rVB3	13145	24384	2.80%	0.325%
13	8.088	2178	2192	2220	rBV	376502	781477	89.67%	10.405%
14	8.844	2415	2427	2455	rBV	445491	746727	85.68%	9.942%
15	10.207	2838	2851	2865	rBV	140587	223976	25.70%	2.982%
16	10.371	2889	2902	2918	rVB2	26361	43818	5.03%	0.583%
17	11.239	3160	3172	3193	rBV	483003	760052	87.21%	10.119%
18	11.612	3276	3288	3313	rBV	436834	685206	78.62%	9.123%
19	12.239	3472	3483	3496	rVB	9218	15165	1.74%	0.202%
20	15.760	4571	4578	4592	rVB2	21140	30914	3.55%	0.412%




Sum of corrected areas: 7510913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029365.D
Acq On : 25 Nov 2022 19:27
Operator : SY/MD
Sample : N5770-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

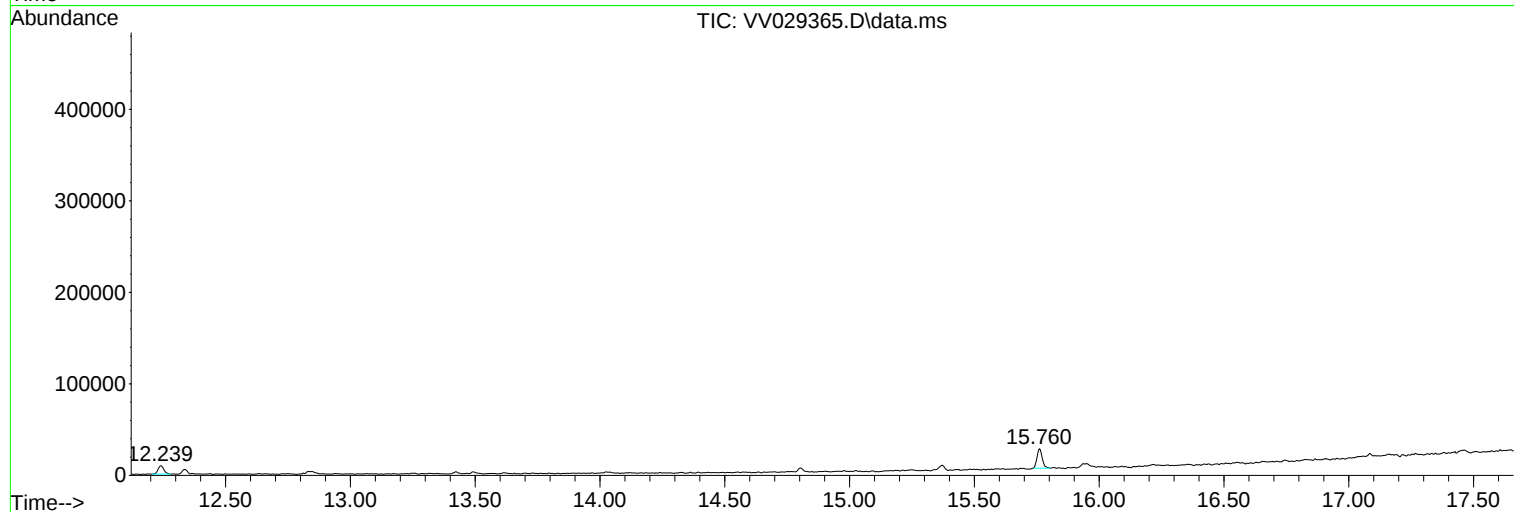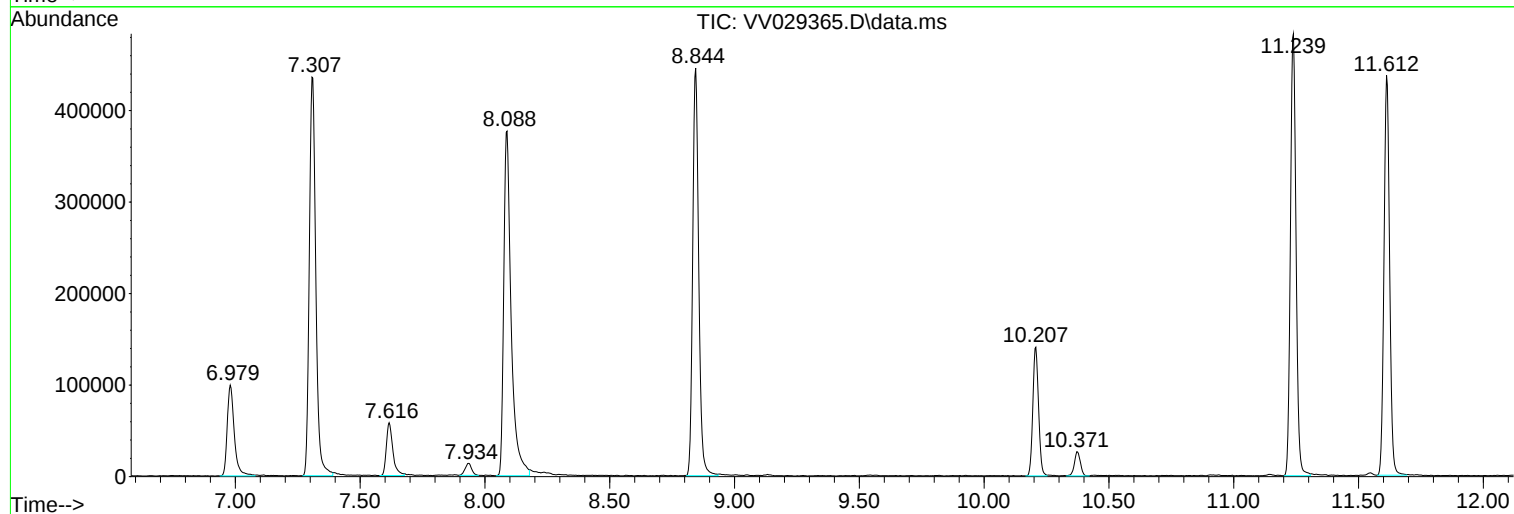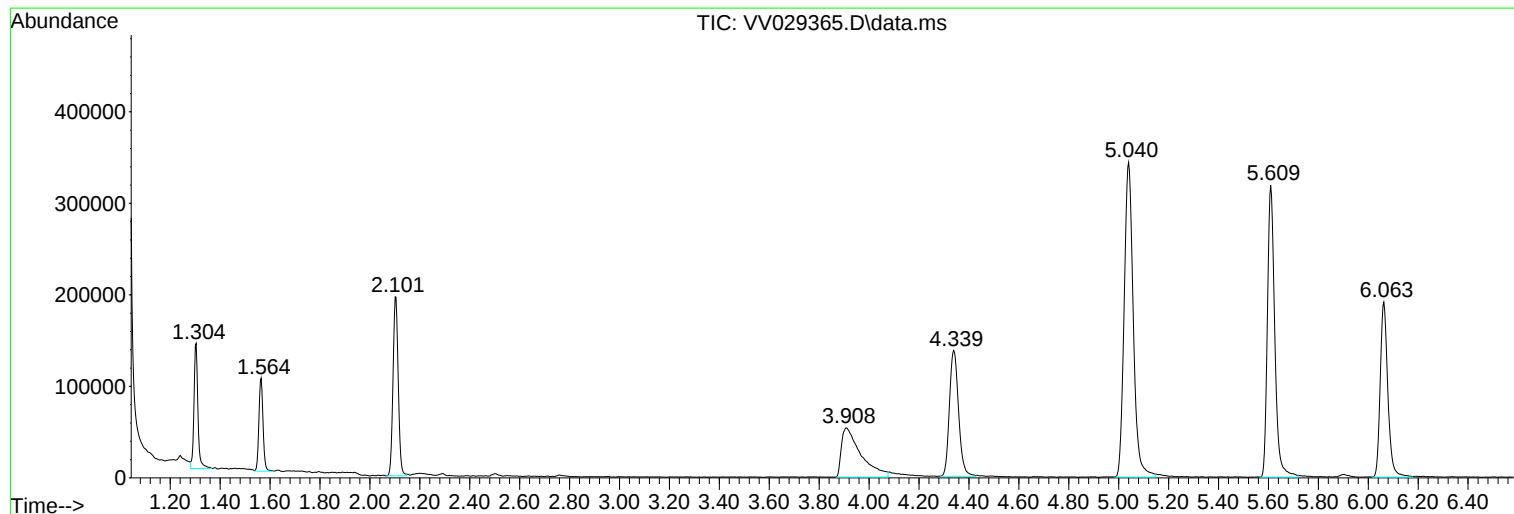

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029365.D
Acq On : 25 Nov 2022 19:27
Operator : SY/MD
Sample : N5770-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029365.D
Acq On : 25 Nov 2022 19:27
Operator : SY/MD
Sample : N5770-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc