

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029367.D
 Acq On : 25 Nov 2022 20:16
 Operator : SY/MD
 Sample : N5759-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB81

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	48	53	58	rBV	17272	17789	2.10%	0.217%
2	1.240	59	62	73	rVV	9099	14094	1.66%	0.172%
3	1.304	75	82	100	rVB	135559	141535	16.70%	1.724%
4	1.565	155	163	176	rVB	99686	113106	13.34%	1.378%
5	2.105	319	331	345	rBV	186395	273847	32.30%	3.335%
6	2.500	446	454	465	rVB	15232	24922	2.94%	0.304%
7	2.757	523	534	551	rBV2	16337	30053	3.55%	0.366%
8	3.915	880	894	946	rBV2	44968	275756	32.53%	3.359%
9	4.339	1009	1026	1060	rBV2	141792	393035	46.36%	4.787%
10	5.040	1226	1244	1284	rBV2	332602	847739	100.00%	10.325%
11	5.609	1407	1421	1446	rBV	313911	643622	75.92%	7.839%
12	5.912	1500	1515	1527	rBV6	13320	29170	3.44%	0.355%
13	6.063	1546	1562	1595	rBV	181324	389911	45.99%	4.749%
14	6.979	1836	1847	1870	rBV	97976	184209	21.73%	2.244%
15	7.307	1937	1949	1963	rBV	414218	748103	88.25%	9.112%
16	7.381	1963	1972	1993	rVB	144056	269139	31.75%	3.278%
17	7.616	2033	2045	2059	rBV	55821	101369	11.96%	1.235%
18	7.969	2147	2155	2169	rVB3	28023	47287	5.58%	0.576%
19	8.088	2180	2192	2228	rBV	353209	748216	88.26%	9.113%
20	8.236	2230	2238	2250	rVV3	21303	42867	5.06%	0.522%
21	8.301	2250	2258	2274	rVB2	19475	38442	4.53%	0.468%
22	8.844	2412	2427	2453	rBV	451020	752067	88.71%	9.160%
23	8.953	2453	2461	2469	rVV3	9062	14513	1.71%	0.177%
24	9.008	2469	2478	2487	rVB	12843	19773	2.33%	0.241%
25	9.130	2504	2516	2532	rBV	41196	69863	8.24%	0.851%
26	9.538	2632	2643	2659	rBV3	19514	42452	5.01%	0.517%
27	9.799	2712	2724	2741	rBV5	9084	18803	2.22%	0.229%
28	10.207	2835	2851	2866	rBV	134559	214726	25.33%	2.615%
29	10.371	2888	2902	2912	rBV3	11538	18786	2.22%	0.229%
30	10.905	3059	3068	3087	rVB2	7550	13706	1.62%	0.167%
31	11.140	3131	3141	3150	rVV3	15734	25579	3.02%	0.312%
32	11.236	3160	3171	3191	rBV	488702	779644	91.97%	9.496%
33	11.333	3193	3201	3213	rVB9	4592	11167	1.32%	0.136%
34	11.542	3246	3266	3277	rBV3	29453	61001	7.20%	0.743%
35	11.612	3277	3288	3311	rVB	419225	665204	78.47%	8.102%
36	12.236	3471	3482	3492	rBV5	8269	16032	1.89%	0.195%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029367.D
Acq On : 25 Nov 2022 20:16
Operator : SY/MD
Sample : N5759-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB81

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Title : TRACE VOA SFAM1.0

37	12.333	3504	3512	3527	rBV3	21741	35011	4.13%	0.426%
38	12.661	3601	3614	3626	rBV2	21204	32762	3.86%	0.399%
39	15.371	4448	4457	4466	rBV2	4877	8478	1.00%	0.103%
40	15.760	4570	4578	4589	rBV2	25635	36490	4.30%	0.444%


Sum of corrected areas: 8210268

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029367.D
Acq On : 25 Nov 2022 20:16
Operator : SY/MD
Sample : N5759-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

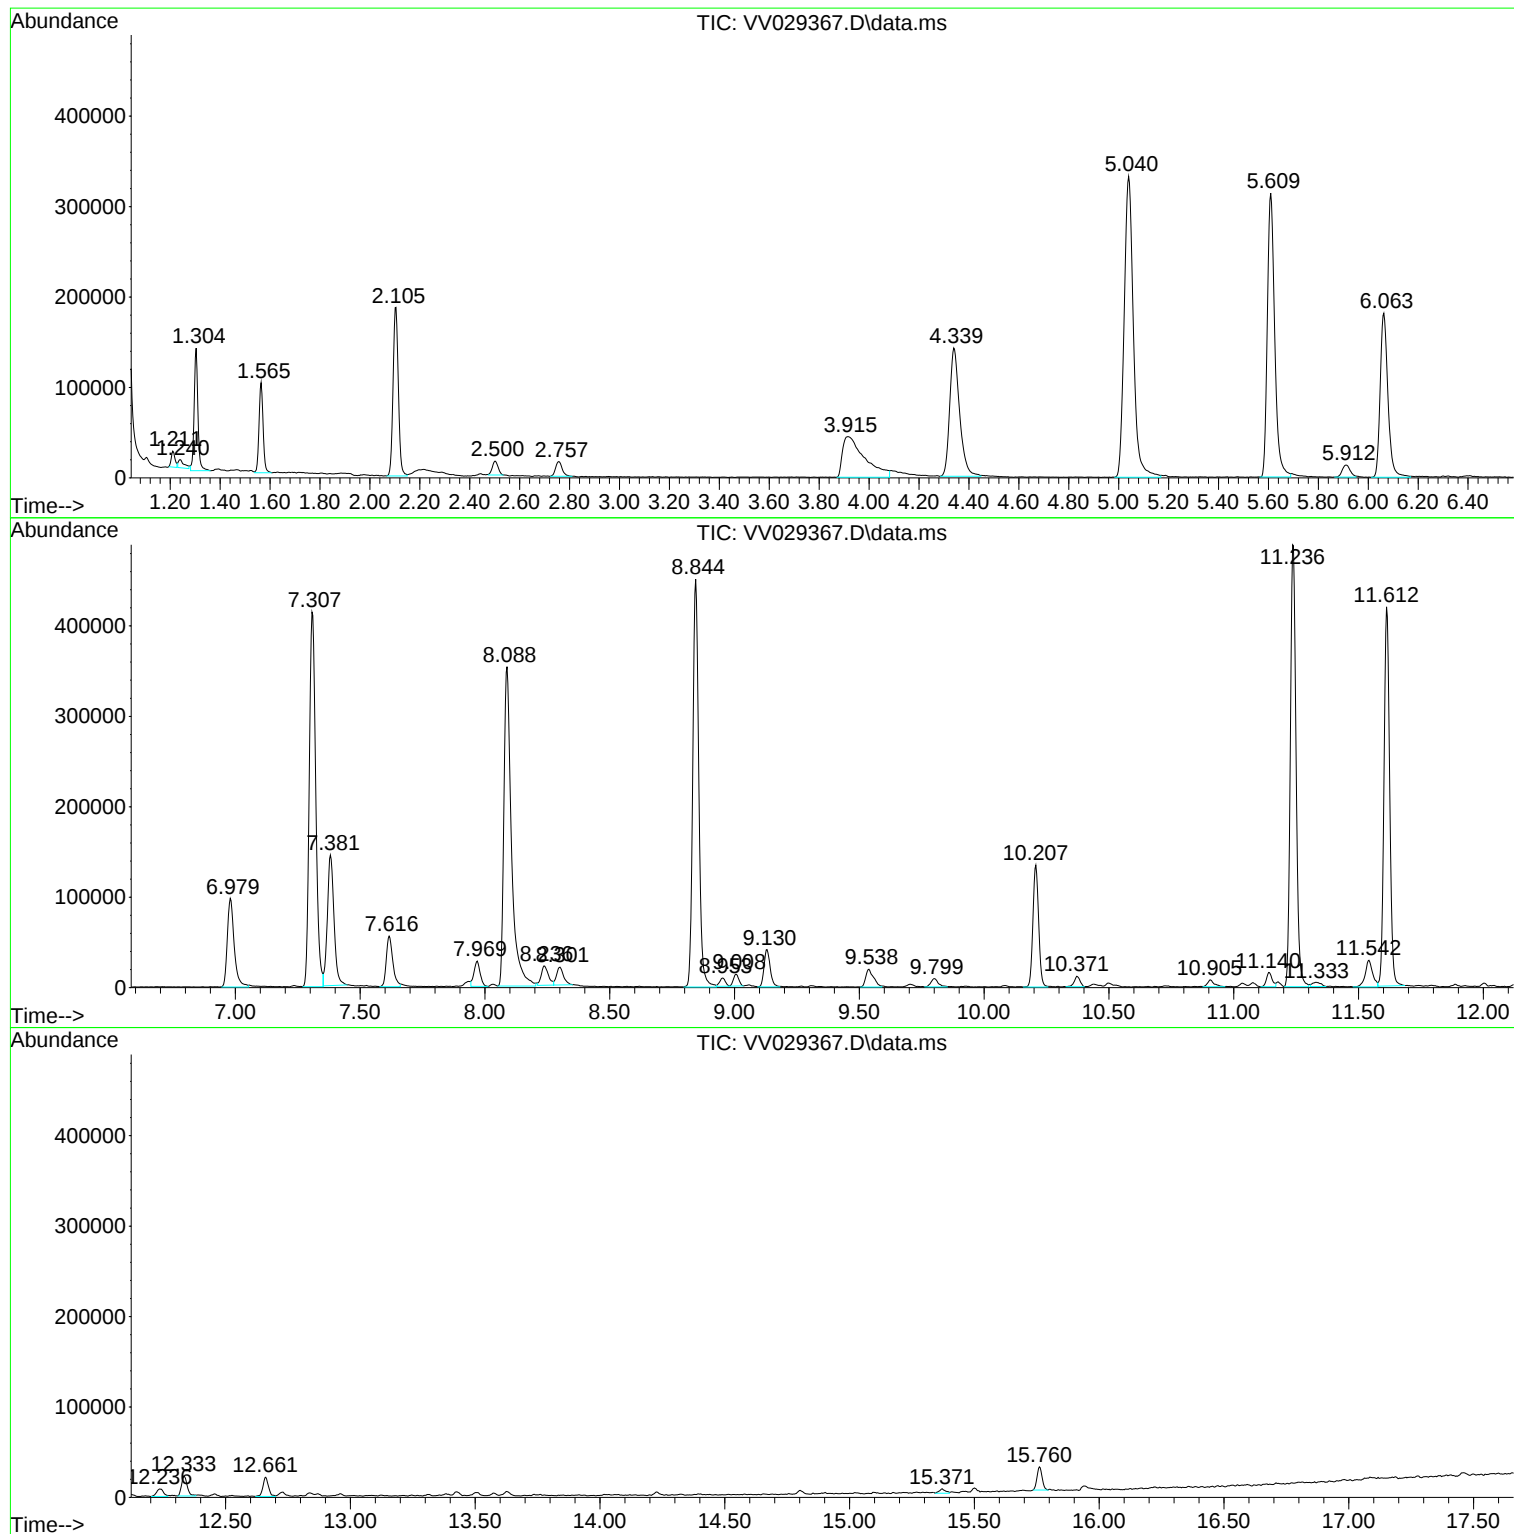

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029367.D
Acq On : 25 Nov 2022 20:16
Operator : SY/MD
Sample : N5759-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
Data File : VV029367.D
Acq On : 25 Nov 2022 20:16
Operator : SY/MD
Sample : N5759-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc