
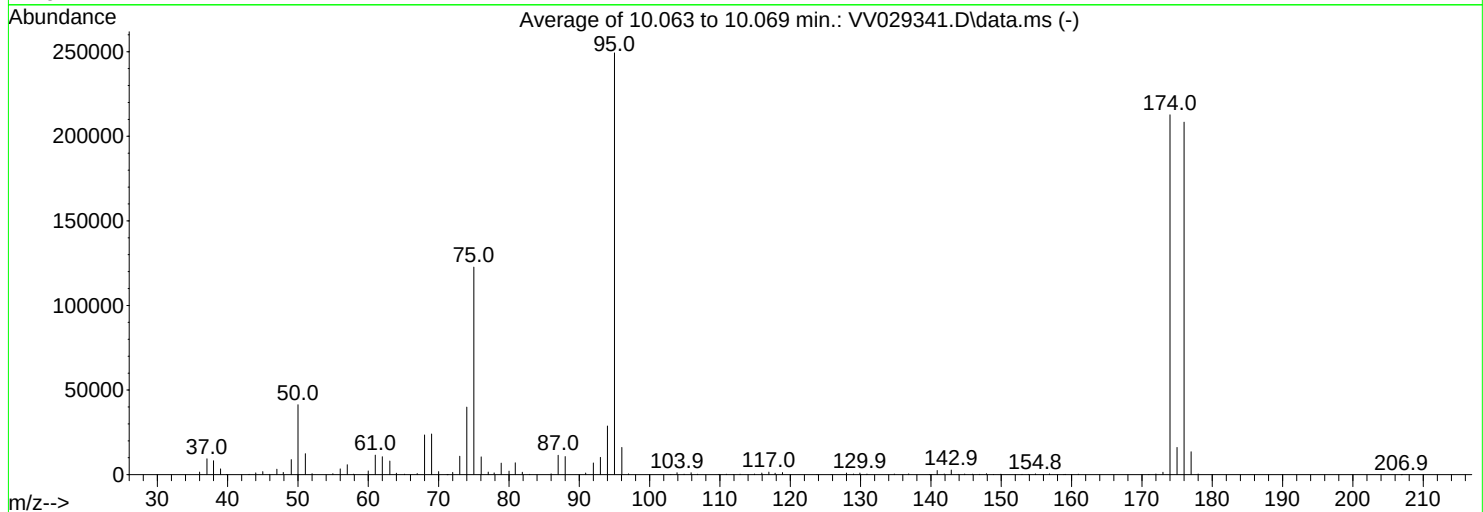


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112522\
 Data File : VV029341.D
 Acq On : 25 Nov 2022 08:44
 Operator : SY/MD
 Sample : BFB205
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB205

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 25 21:27:54 2022

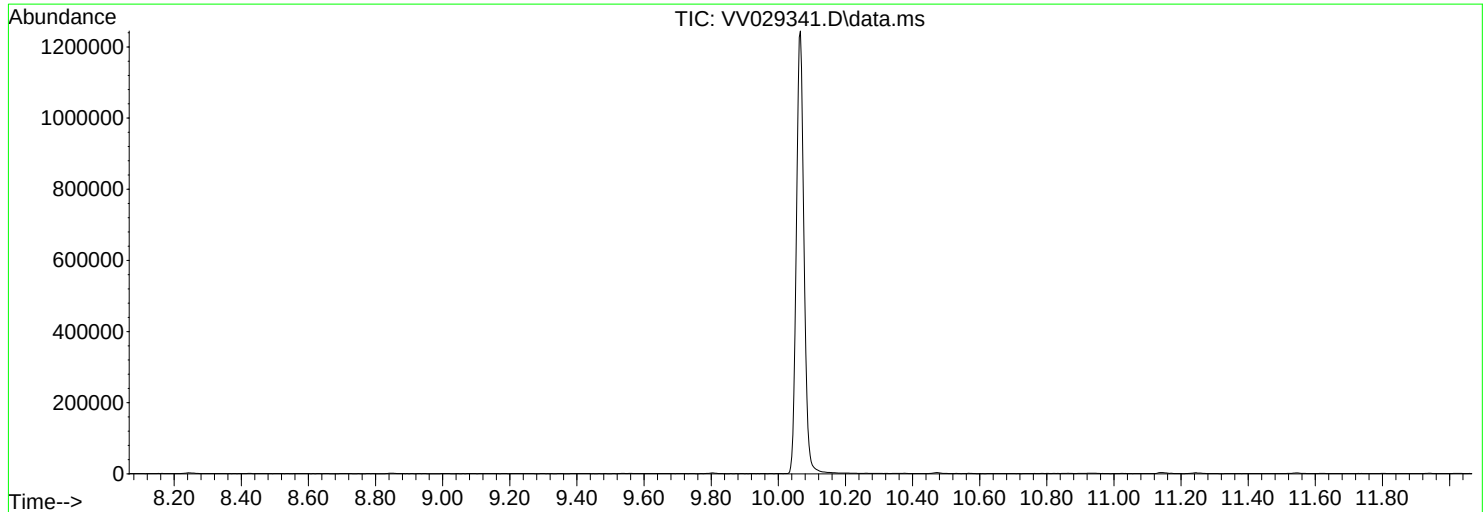

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	41333	PASS
75	95	30	80	49.2	122645	PASS
95	95	100	100	100.0	249323	PASS
96	95	5	9	6.5	16115	PASS
173	174	0.00	2	0.7	1386	PASS
174	95	50	120	85.3	212672	PASS
175	174	5	9	7.6	16062	PASS
176	174	95	105	98.0	208341	PASS
177	176	5	10	6.5	13540	PASS

m/z	Abundance
39.80	232.0
44.00	373.0
207.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1628.0
37.10	9611.0
38.00	8417.0
39.00	3586.0
39.90	292.0
43.00	261.0
44.00	1501.0
45.00	1826.0
46.00	142.0
47.00	3270.0
47.90	1446.0
49.10	9076.0
50.00	43320.0
51.10	12818.0
52.00	610.0
54.90	553.0
56.00	3652.0
57.00	6124.0
57.90	301.0
60.00	2233.0
61.00	12053.0
62.00	10849.0
63.10	8381.0
64.00	952.0
65.10	253.0
67.00	654.0
68.00	24160.0
69.00	24728.0
70.00	1989.0
72.00	1344.0
73.00	11013.0
74.00	40240.0
75.00	127584.0
76.00	10823.0
77.00	1634.0
77.90	997.0
78.90	7120.0
80.00	2254.0
80.90	7133.0
81.90	1544.0
83.00	217.0
86.00	478.0
87.00	11969.0
88.00	11014.0
90.90	1009.0
92.00	7160.0
93.00	10408.0
94.00	29304.0
95.00	255808.0
96.10	16600.0
97.00	426.0
103.00	160.0
103.90	1206.0
104.90	314.0
105.90	1159.0
106.70	258.0
109.90	197.0
110.90	292.0
111.90	131.0
112.90	300.0
114.90	359.0
115.90	974.0
116.90	1520.0
117.80	808.0
118.90	1307.0
123.70	118.0
125.80	125.0
128.00	987.0
129.00	458.0
129.90	983.0
130.90	428.0
134.80	444.0
136.80	405.0
139.80	212.0
140.90	2478.0
141.90	371.0
142.90	2842.0
143.90	175.0
144.80	296.0
145.90	313.0
146.90	195.0
147.90	557.0
148.90	127.0
149.90	244.0
152.00	155.0
152.90	214.0
153.90	166.0
154.90	491.0
156.80	455.0
158.90	303.0
160.90	256.0
171.00	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

173.00	1993.0
174.00	213056.0
175.00	15943.0
176.00	207744.0
177.00	14027.0
178.00	385.0
206.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1587.0
37.00	9731.0
38.00	8500.0
39.00	3584.0
39.90	311.0
43.10	211.0
44.00	1441.0
45.00	1872.0
45.90	155.0
47.00	3344.0
47.90	1433.0
49.10	9052.0
50.00	42696.0
51.10	12767.0
52.00	614.0
55.00	540.0
56.00	3546.0
57.00	6104.0
57.90	281.0
60.00	2222.0
61.00	11992.0
62.00	11014.0
63.00	8309.0
64.00	897.0
65.20	261.0
67.00	688.0
68.00	24096.0
69.00	24712.0
70.00	1820.0
72.00	1322.0
73.00	11299.0
74.00	41312.0
75.00	126648.0
76.00	10889.0
77.00	1564.0
77.90	1089.0
78.90	7020.0
80.00	2213.0
80.90	7211.0
81.90	1488.0
83.00	197.0
86.00	465.0
87.00	11804.0
88.00	10990.0
90.90	961.0
92.00	7129.0
93.00	10510.0
94.00	29864.0
95.00	257792.0
96.00	16672.0
97.00	455.0
103.00	135.0
103.90	1193.0
104.90	299.0
105.90	1156.0
106.80	263.0
109.90	212.0
110.90	269.0
112.00	120.0
112.80	270.0
114.90	366.0
115.90	976.0
116.90	1577.0
117.90	867.0
118.90	1293.0
123.80	143.0
125.80	126.0
128.00	959.0
129.00	442.0
129.90	988.0
130.90	421.0
134.80	435.0
136.90	463.0
140.00	183.0
140.90	2494.0
141.90	392.0
142.90	2831.0
143.90	196.0
144.80	373.0
145.90	336.0
146.90	211.0
147.90	578.0
148.90	151.0
150.00	252.0
152.00	145.0
152.90	202.0
153.90	151.0
154.80	524.0
155.90	113.0
156.90	447.0
159.10	301.0
160.90	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

171.00	144.0
172.10	559.0
173.00	2166.0
174.00	219520.0
175.00	16648.0
176.00	215232.0
177.00	14026.0
178.00	428.0
206.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1387.0
37.00	8814.0
38.00	7805.0
39.00	3142.0
40.00	322.0
43.10	159.0
44.00	1269.0
45.00	1653.0
45.90	163.0
47.00	2960.0
47.90	1245.0
49.00	8439.0
50.00	37984.0
51.00	11729.0
52.00	523.0
55.00	494.0
56.00	3081.0
57.00	5488.0
57.90	232.0
60.00	2053.0
61.00	10525.0
62.00	10074.0
63.00	7545.0
64.00	767.0
65.10	233.0
66.90	640.0
68.00	22232.0
69.00	22544.0
70.00	1567.0
71.20	112.0
72.00	1188.0
73.00	10313.0
74.00	38264.0
75.00	113704.0
76.10	9805.0
77.10	1440.0
77.90	997.0
78.90	6268.0
80.00	1914.0
80.90	6636.0
81.90	1326.0
82.90	207.0
86.00	360.0
87.00	10467.0
88.00	10058.0
90.90	846.0
92.00	6348.0
93.00	9735.0
94.00	27176.0
95.00	234368.0
96.00	15073.0
97.00	468.0
103.90	1051.0
104.90	304.0
105.90	1059.0
106.90	262.0
109.80	216.0
110.90	260.0
111.80	127.0
112.80	220.0
114.90	285.0
116.00	835.0
117.00	1540.0
117.90	803.0
118.90	1101.0
123.90	173.0
125.80	112.0
128.00	829.0
129.00	363.0
129.90	973.0
130.90	344.0
134.80	401.0
136.90	479.0
140.00	160.0
140.90	2381.0
141.90	380.0
142.90	2476.0
143.90	174.0
144.80	403.0
145.90	322.0
146.90	171.0
147.90	573.0
148.90	154.0
150.00	250.0
152.00	115.0
153.00	182.0
153.90	139.0
154.80	543.0
156.00	126.0
156.90	407.0
159.10	273.0
161.00	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

171.00	115.0
171.90	480.0
174.00	205440.0
175.00	15594.0
176.00	202048.0
177.00	12566.0
178.00	387.0
206.90	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205