

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
Quantitation Report (Qedit)




Data File : VV008710.D
Acq On : 26 Nov 2018 12:56
Operator : SY/MD
Sample : VV1126WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK71

Quant Time: Nov 27 03:13:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 27 03:11:05 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
11/27/2018 1:58:00 PM

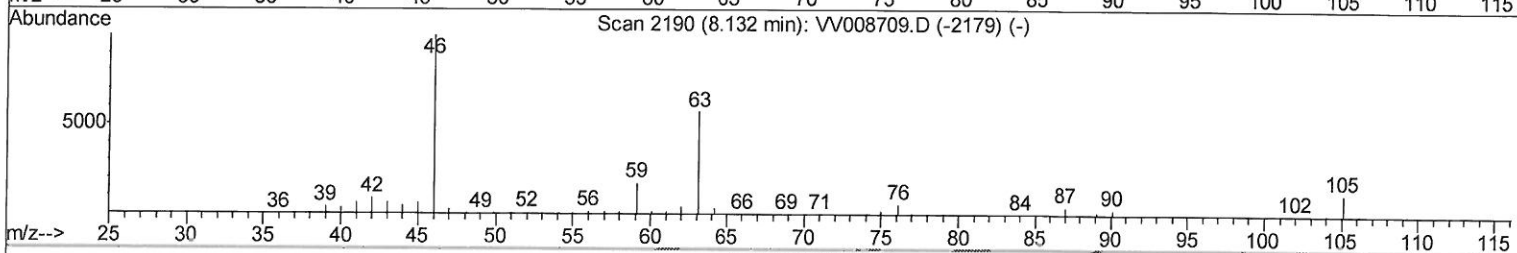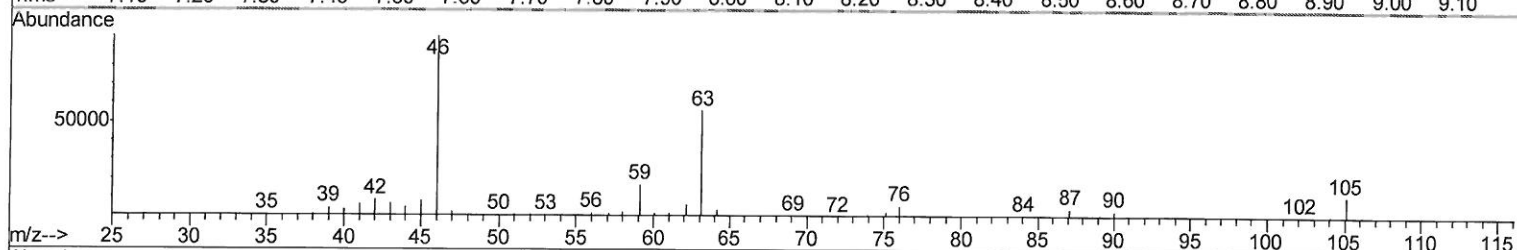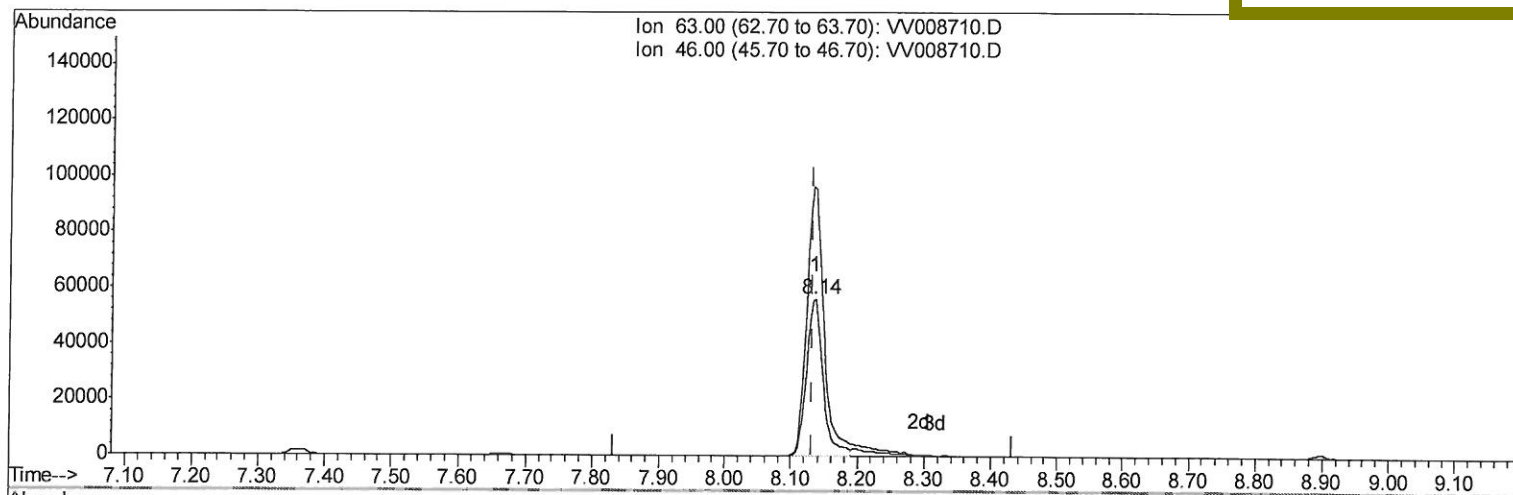

TIC: VV008710.D

(47) 2-Hexanone-d5 (S)

8.135min (+0.003) 79.58ug/L

response 97772

Ion	Exp%	Act%
63.00	100	100
46.00	194.60	186.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
Quantitation Report (Qedit)




Data File : VV008710.D
Acq On : 26 Nov 2018 12:56
Operator : SY/MD
Sample : VV1126WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sample ID :
VBLK71

Quant Time: Nov 27 03:13:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 27 03:11:05 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
11/27/2018 1:58:00 PM

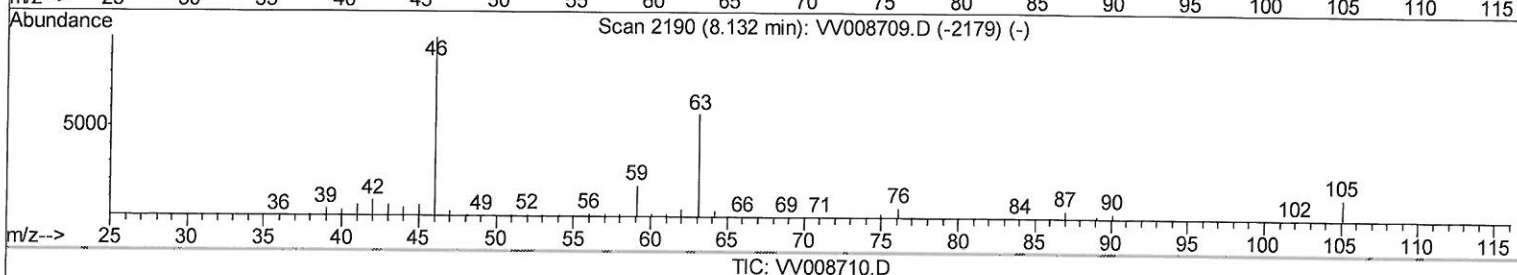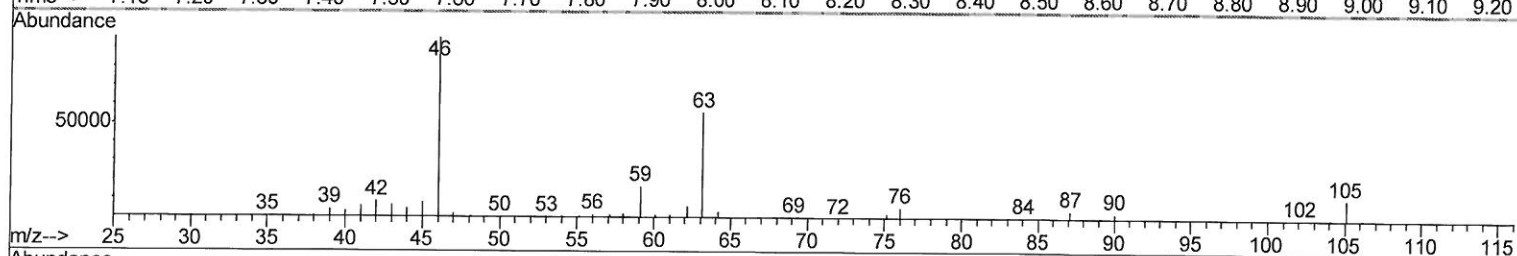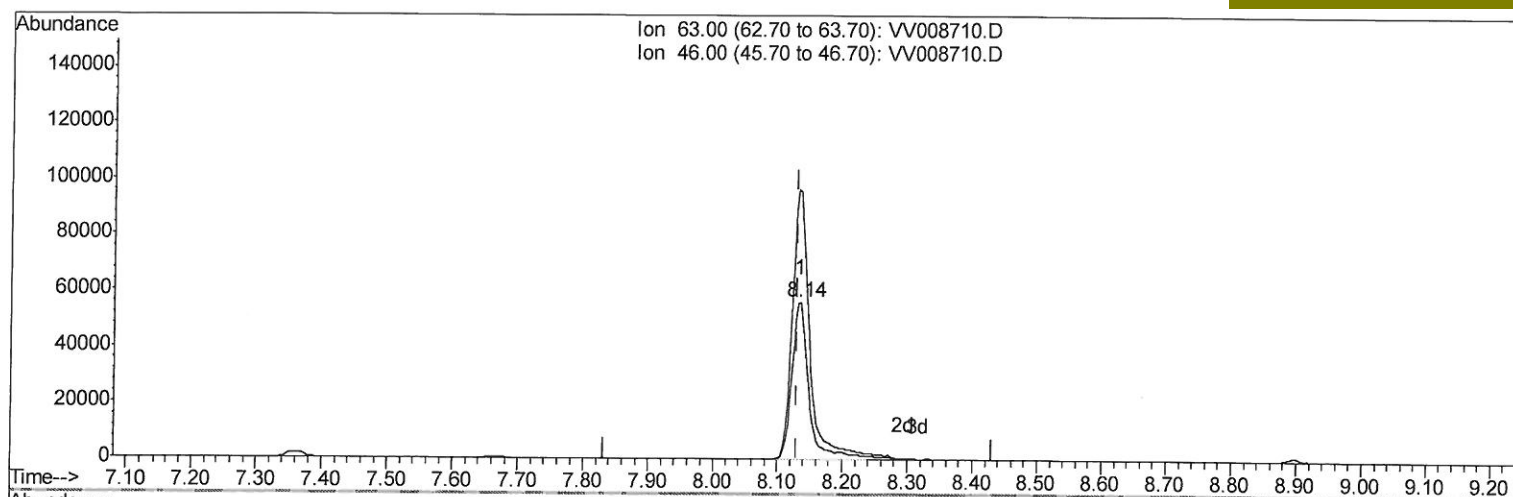

(47) 2-Hexanone-d5 (S)

8.135min (+0.003) 84.07ug/L m

response 103277

Ion	Exp%	Act%
63.00	100	100
46.00	194.60	176.43
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
Quantitation Report (QT Reviewed)

Data File : VV008710.D
Acq On : 26 Nov 2018 12:56
Operator : SY/MD
Sample : VV1126WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK71

Quant Time: Nov 27 03:18:39 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 27 03:11:05 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
11/27/2018 1:58:00 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	302459	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	279425	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	115577	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	90328	42.33	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.66%		
7) Chloroethane-d5	1.59	69	72696	62.37	ug/L	0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	124.74%		
11) 1,1-Dichloroethene-d2	2.13	63	131070	37.22	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.44%		
21) 2-Butanone-d5	3.93	46	152860	87.89	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.89%		
24) Chloroform-d	4.40	84	202006	46.74	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.48%		
26) 1,2-Dichloroethane-d4	5.08	65	133995	48.47	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.94%		
32) Benzene-d6	5.10	84	417942	48.08	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.16%		
36) 1,2-Dichloropropane-d6	6.12	67	132783	48.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.74%		
41) Toluene-d8	7.36	98	376943	48.32	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.64%		
43) trans-1,3-Dichloropropene-	7.66	79	58359	48.02	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.04%		
47) 2-Hexanone-d5	8.14	63	103277m	84.07	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	84.07%		
57) 1,1,2,2-Tetrachloroethane-	10.26	84	161704	43.63	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.26%		
64) 1,2-Dichlorobenzene-d4	11.68	152	129027	51.14	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.28%		

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
Quantitation Report (QT Reviewed)
Data File : VV008710.D
Acq On : 26 Nov 2018 12:56
Operator : SY/MD
Sample : VV1126WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK71

Quant Time: Nov 27 03:18:39 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 27 03:11:05 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
11/27/2018 1:58:00 PM

