

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
 Data File : VV008723.D
 Acq On : 26 Nov 2018 19:50
 Operator : SY/MD
 Sample : J6036-05DL 200X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0928DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	67	72	88	rVB	127802	135386	3.63%	0.976%
2	1.569	143	149	161	rVB	94607	111887	3.00%	0.807%
3	2.129	313	323	335	rBV	221883	312924	8.40%	2.256%
4	2.309	376	379	380	rBV	581	340	0.01%	0.002%
5	2.367	395	397	401	rBV2	325	247	0.01%	0.002%
6	2.463	425	427	428	rBV2	312	99	0.00%	0.001%
7	2.656	479	487	499	rVB2	2177	4314	0.12%	0.031%
8	2.762	517	520	522	rBV	268	175	0.00%	0.001%
9	2.955	574	580	591	rVB2	340	578	0.02%	0.004%
10	3.052	607	610	612	rBV	148	93	0.00%	0.001%
11	3.064	612	614	616	rBV	242	126	0.00%	0.001%
12	3.177	646	649	651	rBV	410	290	0.01%	0.002%
13	3.254	671	673	676	rBV	183	59	0.00%	0.000%
14	3.437	728	730	732	rBV2	148	91	0.00%	0.001%
15	3.508	749	752	757	rVB	124	79	0.00%	0.001%
16	3.534	758	760	768	rVV2	269	304	0.01%	0.002%
17	3.576	769	773	780	rVB	275	287	0.01%	0.002%
18	3.627	786	789	791	rBV	167	104	0.00%	0.001%
19	3.672	800	803	807	rVB2	193	123	0.00%	0.001%
20	3.691	807	809	812	rVB2	207	114	0.00%	0.001%
21	3.711	812	815	819	rBV2	319	294	0.01%	0.002%
22	3.778	834	836	839	rBV2	180	129	0.00%	0.001%
23	3.807	841	845	848	rBV3	625	625	0.02%	0.005%
24	3.859	857	861	863	rBV	269	214	0.01%	0.002%
25	3.933	869	884	911	rBV	93414	243177	6.53%	1.753%
26	4.405	1015	1031	1056	rBV	179428	433235	11.63%	3.123%
27	4.566	1079	1081	1084	rBV2	264	186	0.00%	0.001%
28	4.582	1084	1086	1087	rBV	165	50	0.00%	0.000%
29	4.611	1093	1095	1100	rVB	437	269	0.01%	0.002%
30	4.637	1100	1103	1107	rVB3	433	300	0.01%	0.002%
31	4.688	1113	1119	1123	rBV3	221	232	0.01%	0.002%
32	4.727	1129	1131	1134	rVB2	396	180	0.00%	0.001%
33	4.788	1147	1150	1154	rVB	220	140	0.00%	0.001%
34	4.814	1155	1158	1160	rBV2	133	85	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
 Data File : VV008723.D
 Acq On : 26 Nov 2018 19:50
 Operator : SY/MD
 Sample : J6036-05DL 200X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0928DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
 Title : VOC Analysis

35	4.881	1170	1179	1188	rVB5	1490	2694	0.07%	0.019%
36	4.916	1188	1190	1191	rBV5	223	84	0.00%	0.001%
37	4.945	1197	1199	1200	rBV	149	45	0.00%	0.000%
38	5.016	1218	1221	1226	rVB2	212	193	0.01%	0.001%
39	5.100	1226	1247	1257	rBV2	451493	1129476	30.32%	8.142%
40	5.418	1343	1346	1349	rBV2	255	214	0.01%	0.002%
41	5.537	1380	1383	1390	rBV4	418	435	0.01%	0.003%
42	5.569	1390	1393	1395	rBV2	211	160	0.00%	0.001%
43	5.666	1408	1423	1448	rBV	338680	664647	17.84%	4.791%
44	5.949	1501	1511	1524	rBV5	5995	11344	0.30%	0.082%
45	5.997	1524	1526	1529	rVB3	152	68	0.00%	0.000%
46	6.039	1538	1539	1541	rBV	280	122	0.00%	0.001%
47	6.061	1544	1546	1550	rVB2	403	197	0.01%	0.001%
48	6.122	1550	1565	1590	rBV	248820	505029	13.56%	3.640%
49	6.309	1620	1623	1625	rBV	325	183	0.00%	0.001%
50	6.421	1655	1658	1663	rVB2	208	193	0.01%	0.001%
51	6.450	1663	1667	1670	rVB2	201	148	0.00%	0.001%
52	6.466	1670	1672	1676	rVB2	154	105	0.00%	0.001%
53	6.489	1676	1679	1681	rBV	368	197	0.01%	0.001%
54	6.823	1782	1783	1784	rBV	227	59	0.00%	0.000%
55	6.836	1784	1787	1788	rBV2	168	104	0.00%	0.001%
56	6.862	1794	1795	1798	rBV	132	50	0.00%	0.000%
57	7.032	1834	1848	1866	rBV	132004	235551	6.32%	1.698%
58	7.260	1917	1919	1921	rBV2	287	165	0.00%	0.001%
59	7.363	1936	1951	1968	rBV	516200	901369	24.20%	6.497%
60	7.595	2020	2023	2025	rBV	238	115	0.00%	0.001%
61	7.666	2034	2045	2063	rBV	94585	157408	4.23%	1.135%
62	7.871	2107	2109	2113	rBV2	280	204	0.01%	0.001%
63	8.071	2170	2171	2174	rVB	357	102	0.00%	0.001%
64	8.132	2178	2190	2219	rBV	280667	509586	13.68%	3.673%
65	8.379	2265	2267	2271	rVB2	464	271	0.01%	0.002%
66	8.402	2271	2274	2276	rVB	278	165	0.00%	0.001%
67	8.440	2284	2286	2291	rBV2	390	382	0.01%	0.003%
68	8.508	2304	2307	2311	rVB2	335	222	0.01%	0.002%
69	8.604	2333	2337	2340	rBV2	284	235	0.01%	0.002%
70	8.781	2388	2392	2394	rBV	297	236	0.01%	0.002%
71	8.926	2415	2437	2480	rBV2	1812497	3725183	100.00%	26.852%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
 Data File : VV008723.D
 Acq On : 26 Nov 2018 19:50
 Operator : SY/MD
 Sample : J6036-05DL 200X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0928DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
 Title : VOC Analysis

72	9.093	2486	2489	2491	rBV2	201	132	0.00%	0.001%
73	9.212	2522	2526	2529	rBV	179	189	0.01%	0.001%
74	9.344	2563	2567	2571	rBV	301	284	0.01%	0.002%
75	9.405	2583	2586	2590	rVB2	287	226	0.01%	0.002%
76	9.447	2595	2599	2605	rBV	278	310	0.01%	0.002%
77	9.733	2685	2688	2694	rVB	266	238	0.01%	0.002%
78	9.932	2748	2750	2753	rVB2	195	100	0.00%	0.001%
79	10.219	2835	2839	2841	rBV2	248	202	0.01%	0.001%
80	10.264	2841	2853	2873	rVV	322501	506350	13.59%	3.650%
81	10.591	2954	2955	2959	rBV2	229	145	0.00%	0.001%
82	11.228	3142	3153	3163	rBV2	70479	111710	3.00%	0.805%
83	11.318	3164	3181	3201	rVB2	709768	1752521	47.05%	12.633%
84	11.691	3279	3297	3319	rBV2	1104253	2298111	61.69%	16.565%
85	11.807	3331	3333	3335	rBV	282	122	0.00%	0.001%
86	13.315	3792	3802	3815	rBV	57694	91062	2.44%	0.656%
87	13.797	3944	3952	3963	rVB3	12620	17504	0.47%	0.126%


Sum of corrected areas: 13872883

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
Data File : VV008723.D
Acq On : 26 Nov 2018 19:50
Operator : SY/MD
Sample : J6036-05DL 200X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0928DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

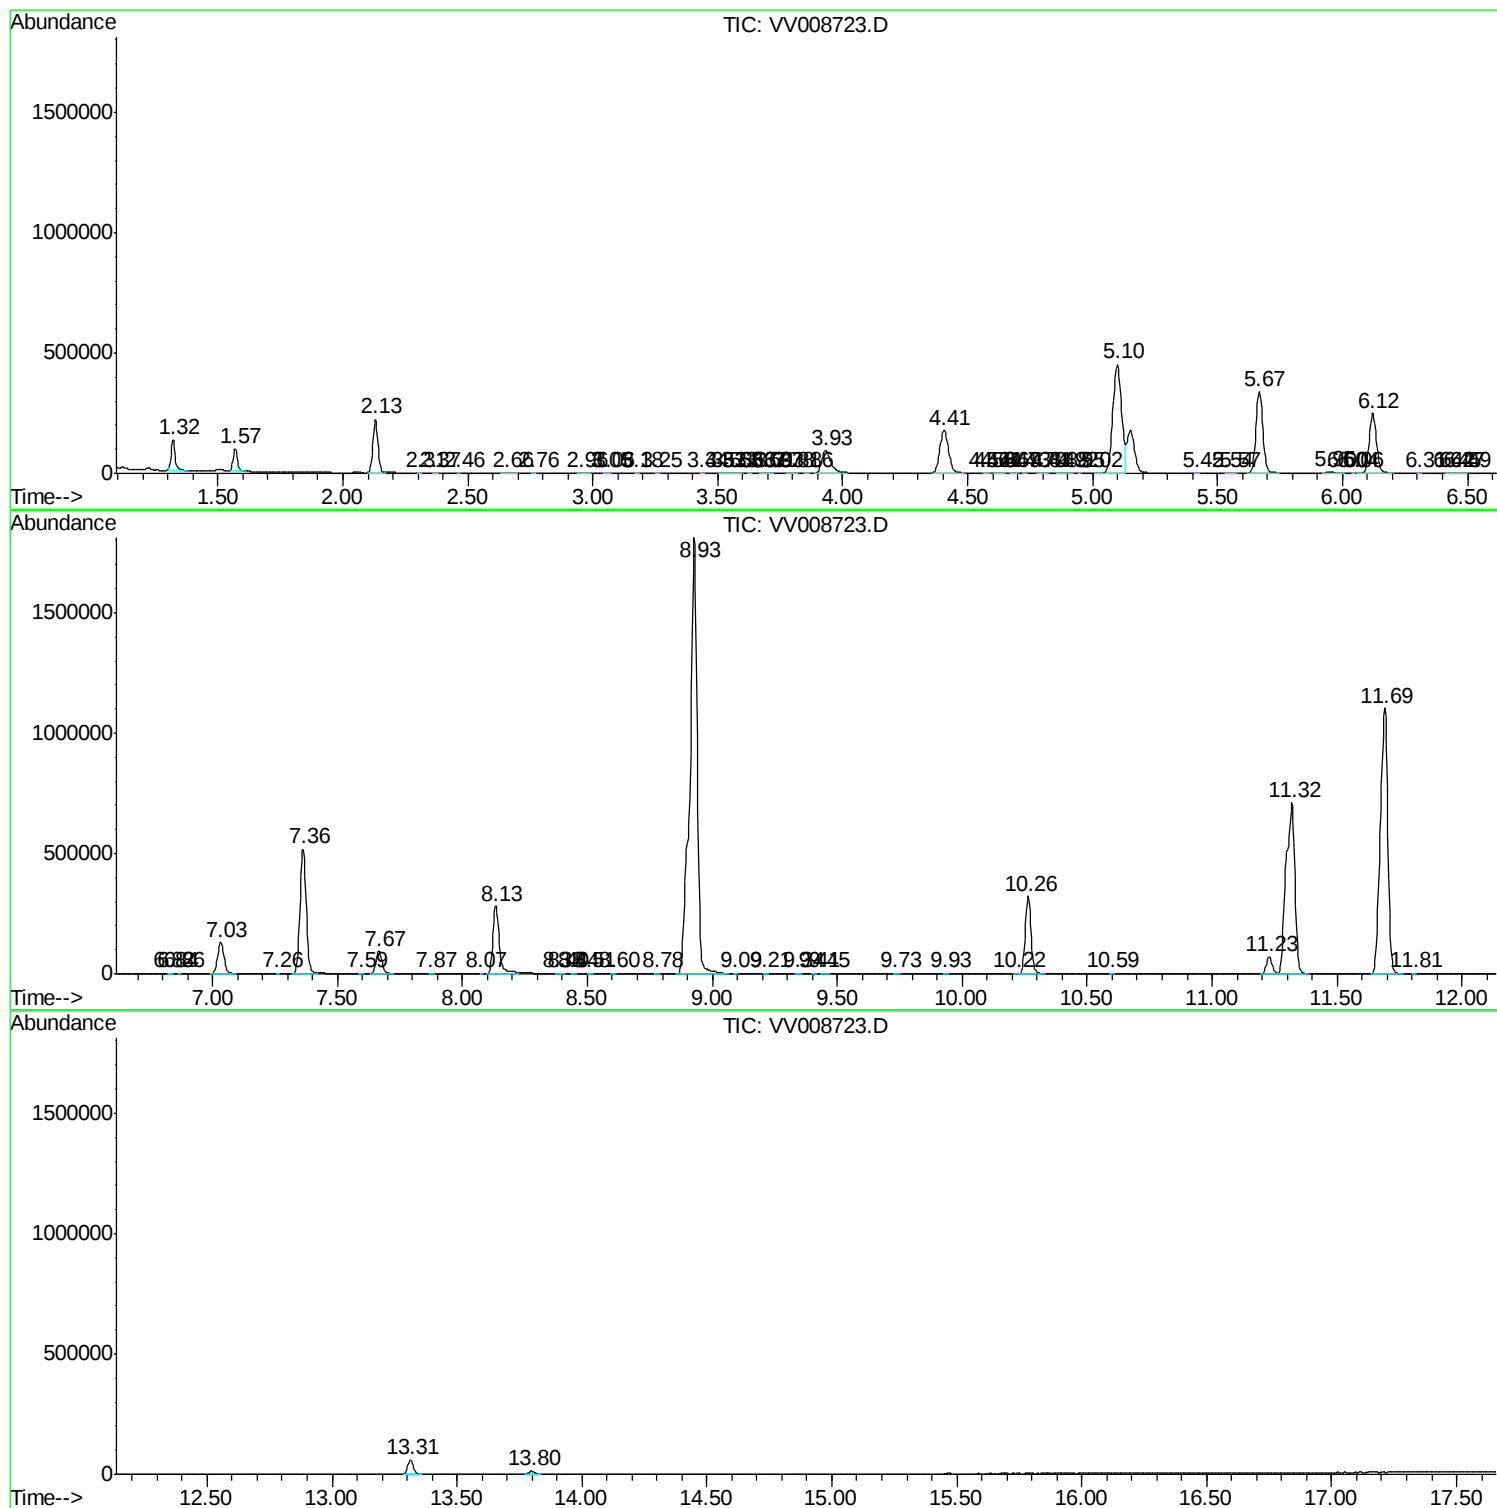

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
Data File : VV008723.D
Acq On : 26 Nov 2018 19:50
Operator : SY/MD
Sample : J6036-05DL 200X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0928DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112618\
Data File : VV008723.D
Acq On : 26 Nov 2018 19:50
Operator : SY/MD
Sample : J6036-05DL 200X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0928DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc