


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112618\
Data File : VV008708.D
Acq On : 26 Nov 2018 11:29
Operator : SY/MD
Sample : BFB49
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Title : VOC Analysis
Last Update : Tue Nov 27 03:11:05 2018

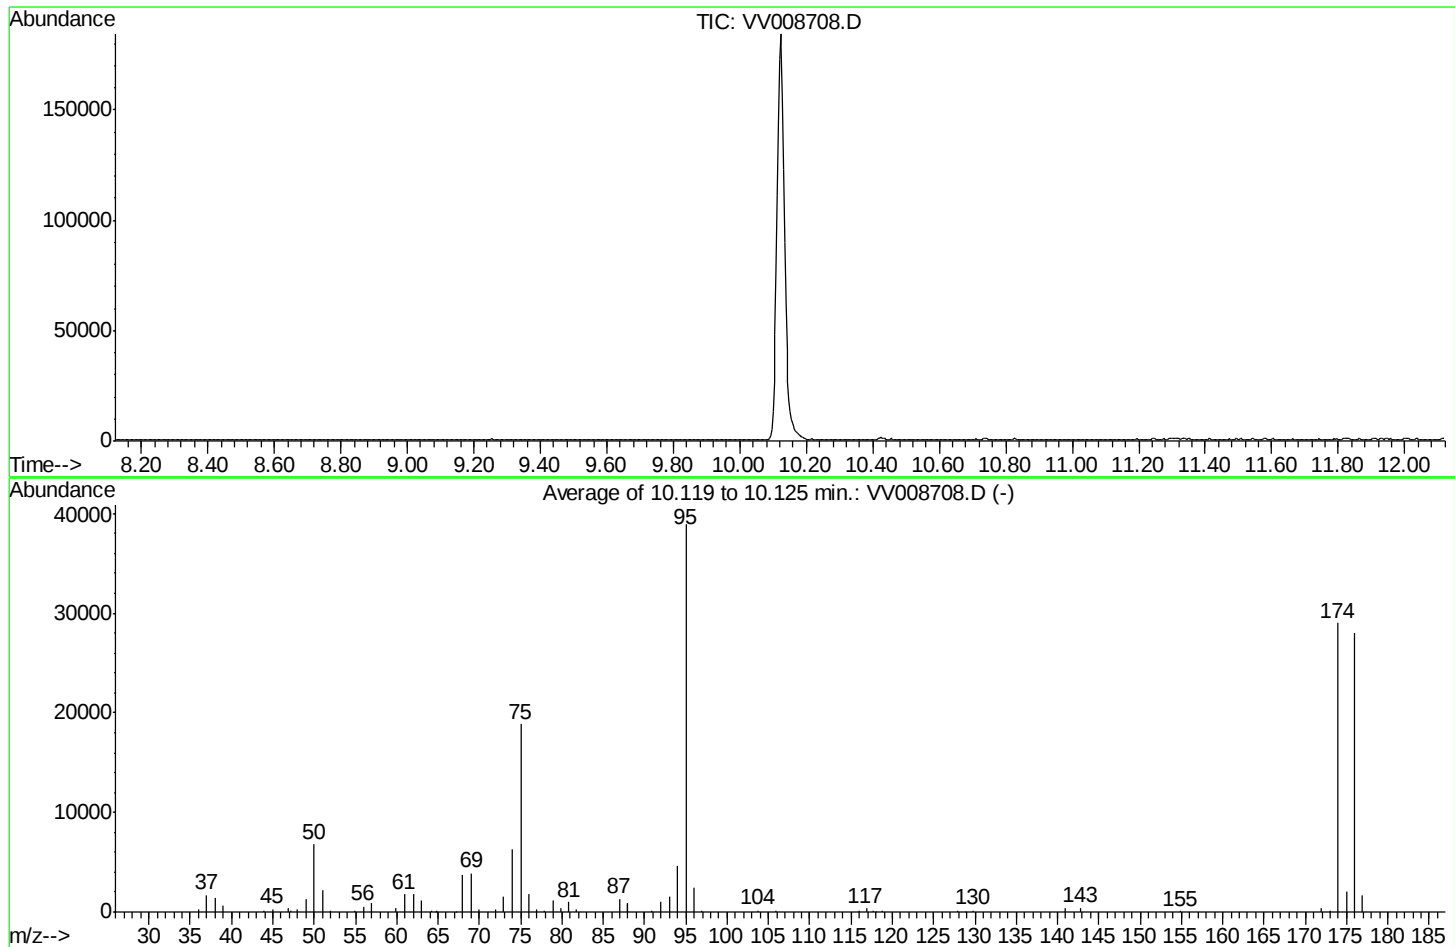

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	6769	PASS
75	95	30	80	48.5	18866	PASS
95	95	100	100	100.0	38912	PASS
96	95	5	9	6.3	2449	PASS
173	174	0.00	2	0.4	127	PASS
174	95	50	120	74.5	28997	PASS
175	174	5	9	7.2	2076	PASS
176	174	95	101	96.5	27973	PASS
177	176	5	9	6.0	1682	PASS

m/z	Abundance
39.90	273.0
44.00	495.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	292.0
37.00	1703.0
38.00	1414.0
39.00	547.0
40.00	232.0
43.90	560.0
45.00	259.0
46.90	444.0
48.00	296.0
49.00	1238.0
50.00	6814.0
51.00	2001.0
52.00	130.0
54.90	129.0
56.00	491.0
57.00	977.0
60.00	413.0
60.90	1626.0
62.10	1622.0
63.00	1128.0
64.90	261.0
68.00	3670.0
69.10	3815.0
70.00	276.0
71.90	264.0
73.00	1573.0
74.00	6506.0
75.00	18768.0
76.00	1796.0
77.00	197.0
77.80	118.0
78.90	1273.0
79.90	319.0
80.80	934.0
81.80	279.0
86.90	1271.0
88.00	1412.0
90.80	168.0
92.00	1007.0
93.00	1549.0
94.00	4598.0
95.00	38824.0
96.00	2305.0
96.80	106.0
103.80	203.0
105.90	157.0
116.00	122.0
116.90	345.0
118.00	139.0
118.80	184.0
127.90	168.0
129.80	147.0
140.90	388.0
142.80	434.0
154.90	129.0
171.90	302.0
173.00	383.0
174.00	29616.0
175.00	1944.0
176.00	28680.0
176.90	1561.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	357.0
37.00	1802.0
38.00	1506.0
39.00	649.0
39.90	208.0
43.90	574.0
45.00	296.0
46.90	381.0
48.00	265.0
49.00	1370.0
50.00	6988.0
51.00	2348.0
52.00	116.0
54.90	137.0
56.00	546.0
57.00	960.0
59.90	370.0
60.90	1846.0
62.00	1825.0
63.00	1160.0
64.20	100.0
64.90	177.0
68.00	3855.0
69.00	3994.0
70.00	261.0
71.90	272.0
72.90	1647.0
74.00	6558.0
75.00	19456.0
76.00	1918.0
76.90	237.0
77.80	108.0
78.90	1250.0
79.90	406.0
80.80	1008.0
81.80	291.0
86.90	1334.0
87.90	1310.0
90.80	183.0
92.00	994.0
93.00	1631.0
94.00	4791.0
95.00	40344.0
96.10	2535.0
96.90	137.0
103.80	181.0
105.80	173.0
116.00	121.0
116.90	340.0
117.70	140.0
118.80	200.0
127.90	136.0
128.90	103.0
129.80	145.0
140.90	394.0
142.80	429.0
154.90	119.0
171.90	354.0
174.00	30136.0
175.00	2131.0
176.00	28992.0
177.00	1768.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	319.0
37.00	1706.0
38.00	1428.0
39.00	629.0
39.90	205.0
44.00	610.0
44.90	294.0
46.90	296.0
47.10	255.0
48.00	190.0
49.00	1399.0
50.00	6505.0
51.00	2309.0
52.10	111.0
54.80	156.0
56.00	561.0
57.00	951.0
59.90	337.0
61.00	1846.0
62.00	1778.0
63.00	1158.0
64.20	154.0
64.70	126.0
67.10	127.0
68.00	3681.0
69.00	3812.0
70.00	254.0
72.00	247.0
72.90	1564.0
74.00	6008.0
75.00	18376.0
76.00	1816.0
76.90	256.0
78.90	1138.0
79.90	414.0
80.90	1006.0
81.80	244.0
87.00	1308.0
87.90	1126.0
88.00	1136.0
90.80	177.0
92.00	937.0
93.00	1611.0
94.00	4412.0
95.00	37568.0
96.10	2507.0
97.00	139.0
103.80	151.0
105.80	188.0
116.00	110.0
116.90	305.0
117.70	141.0
118.80	208.0
129.80	123.0
141.00	394.0
142.80	403.0
172.00	386.0
174.00	27240.0
174.90	2153.0
176.00	26248.0
177.00	1717.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49