


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112619\
Data File : VV013801.D
Acq On : 26 Nov 2019 21:15
Operator : SY/MD
Sample : K6056-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFE08

Manual Integrations
APPROVED

MMDadoda
11/27/2019 11:40:31 AM

Quant Time: Nov 27 04:21:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 27 03:09:16 2019
Response via : Initial Calibration

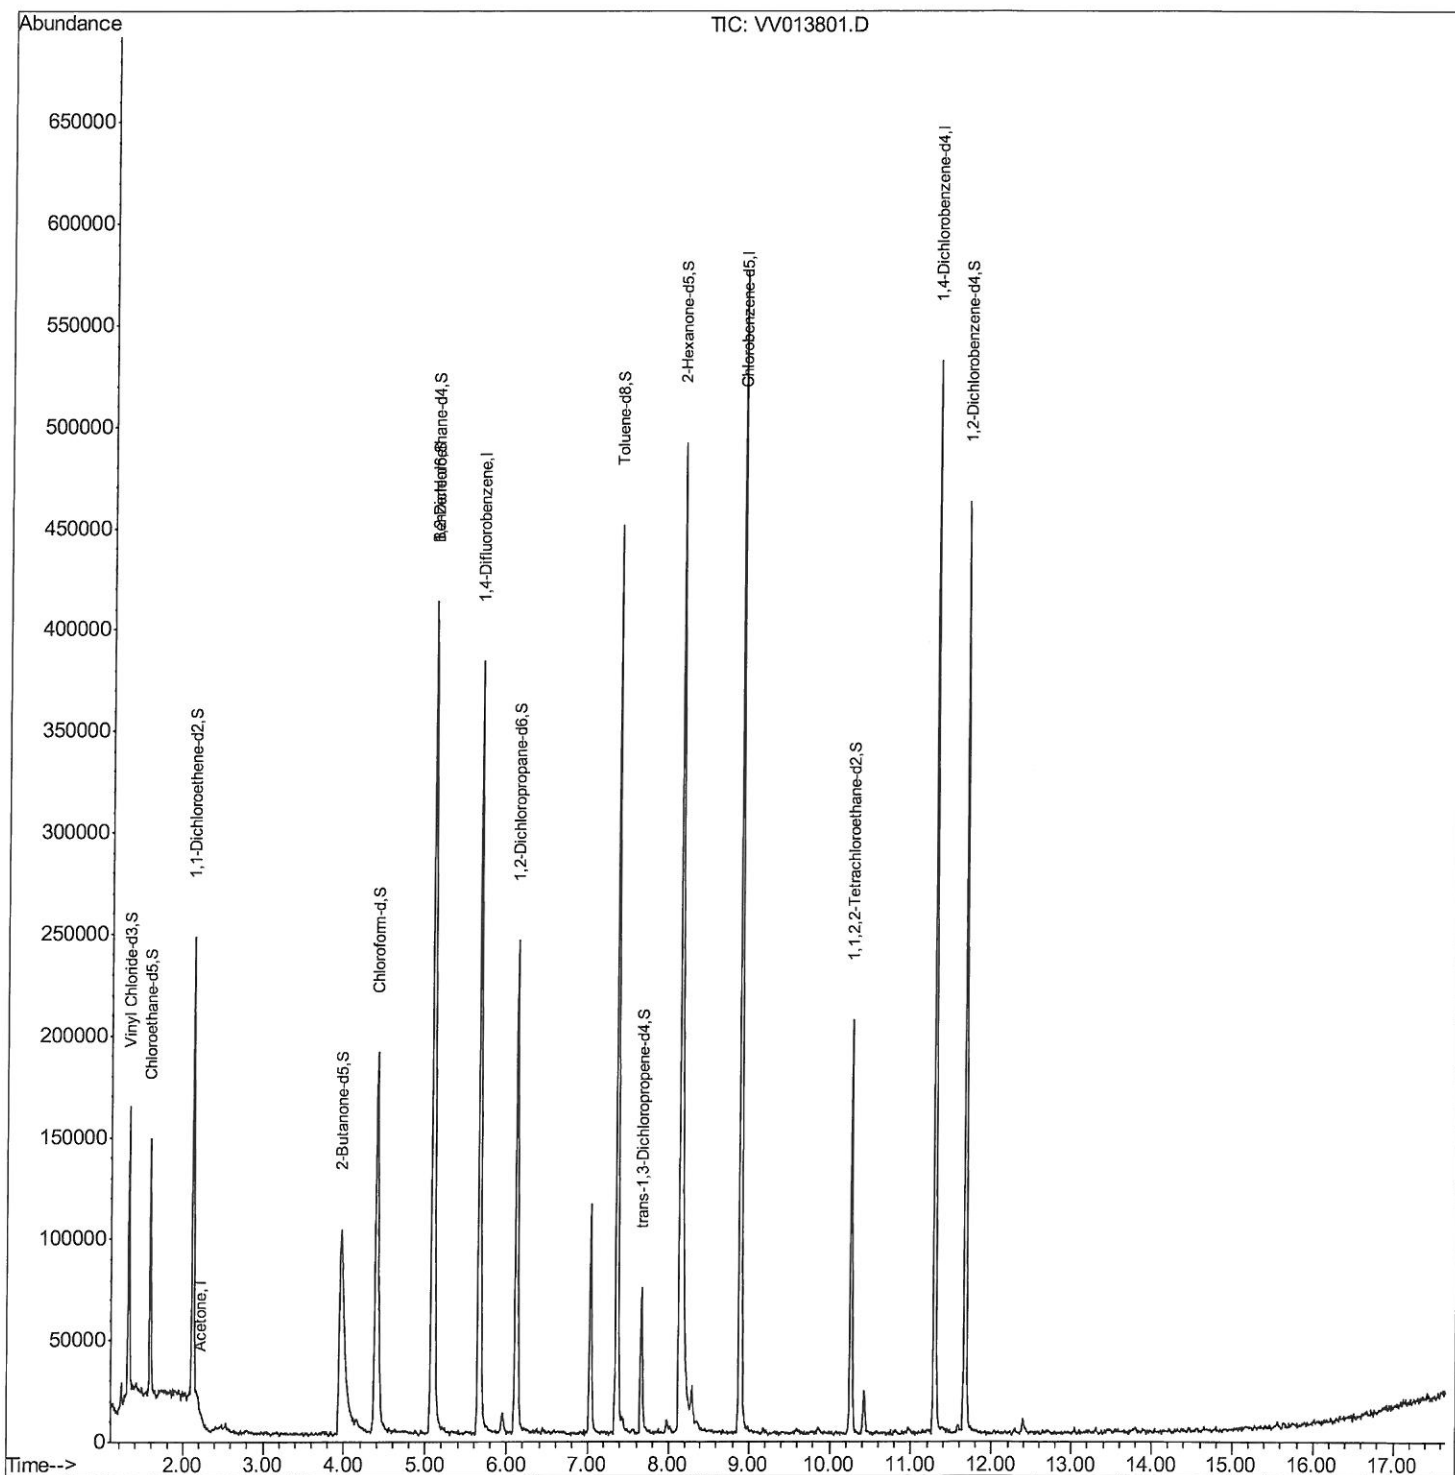

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112619\
 Data File : VV013801.D
 Acq On : 26 Nov 2019 21:15
 Operator : SY/MD
 Sample : K6056-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 BFE08

Manual Integrations
APPROVED

MMDadoda
 11/27/2019 11:40:31 AM

Quant Time: Nov 27 03:13:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 27 03:09:16 2019
 Response via : Initial Calibration

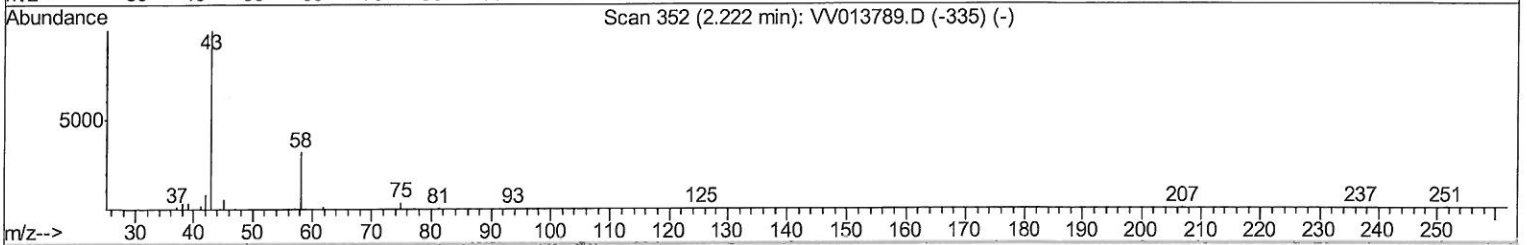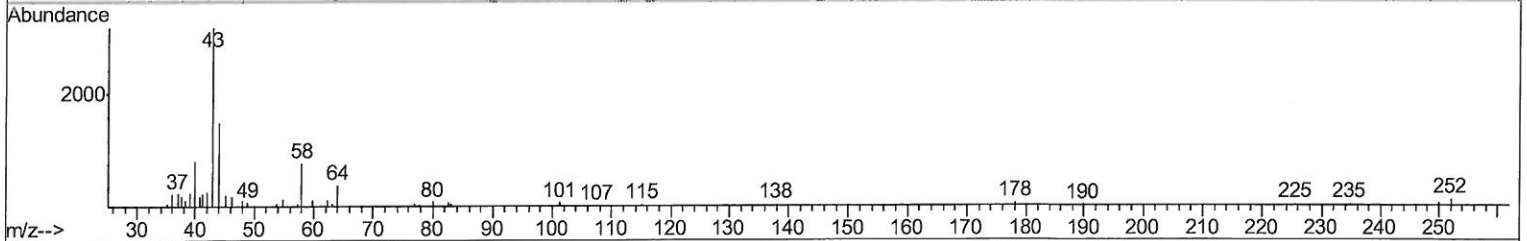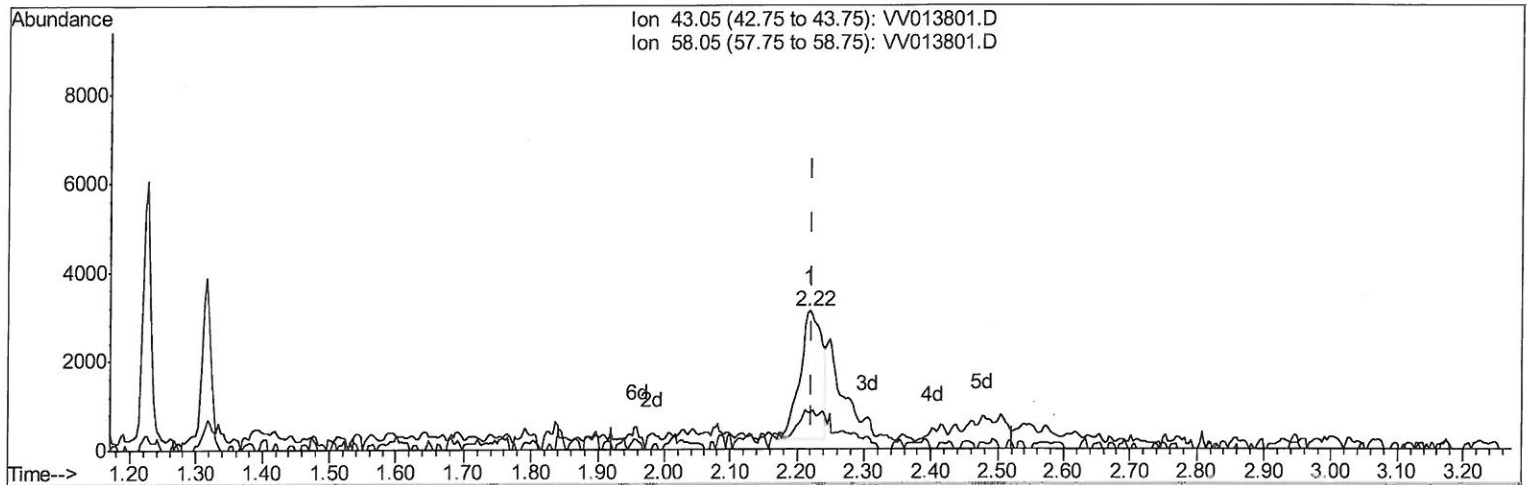

TIC: VV013801.D

(13) Acetone (T)

2.219min (-0.003) 2.20ug/L

response 6542

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	10.44
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112619\
 Data File : VV013801.D
 Acq On : 26 Nov 2019 21:15
 Operator : SY/MD
 Sample : K6056-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 BFE08

Manual Integrations
APPROVED

MMDadoda
 11/27/2019 11:40:31 AM

Quant Time: Nov 27 03:13:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 27 03:09:16 2019
 Response via : Initial Calibration

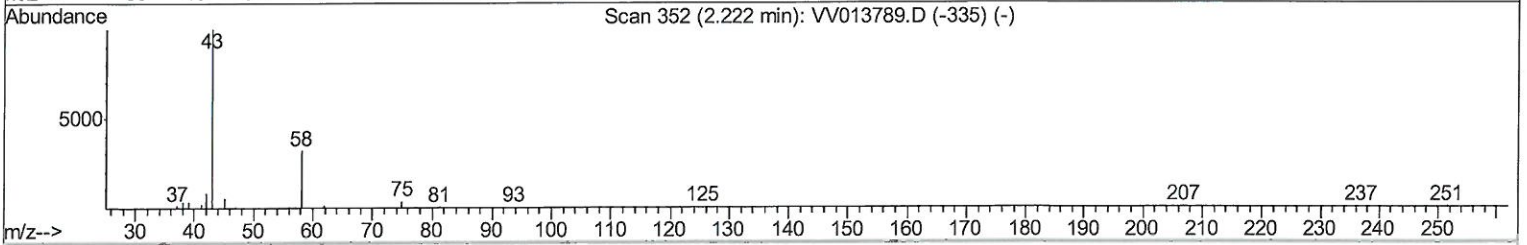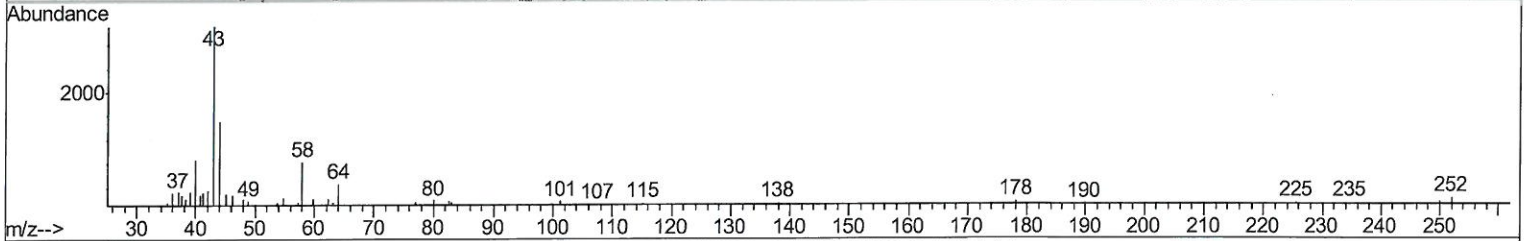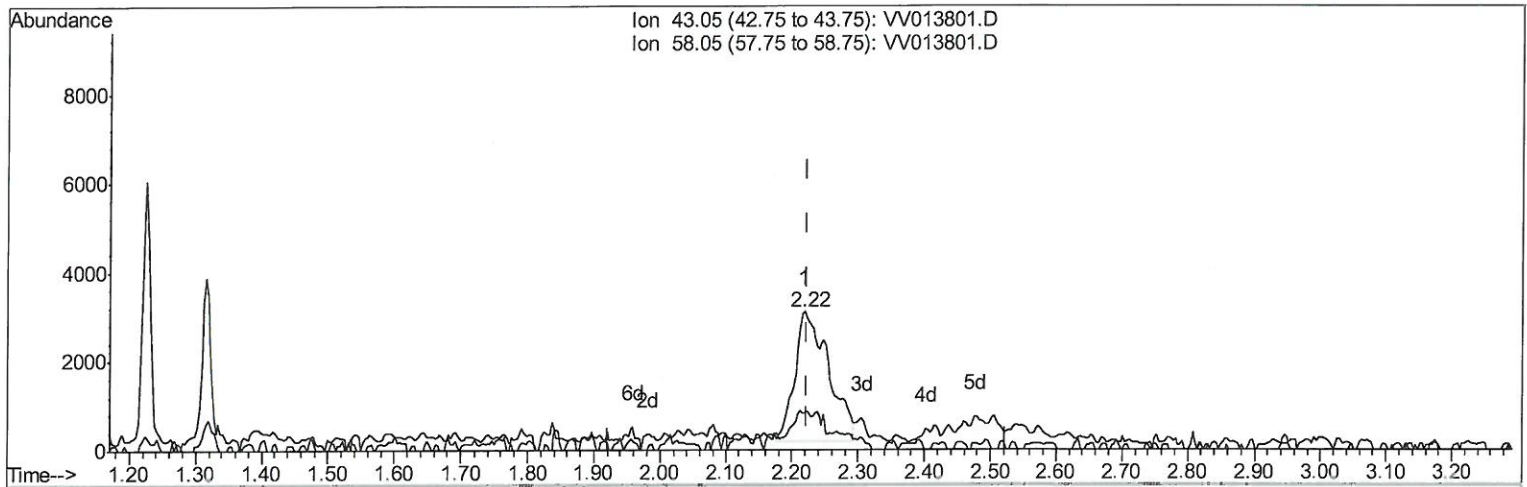

TIC: VV013801.D

(13) Acetone (T)

2.219min (-0.003) 3.49ug/L m

response 10397

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	6.57
0.00	0.00	0.00
0.00	0.00	0.00

MD
11/27/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112619\
 Data File : VV013801.D
 Acq On : 26 Nov 2019 21:15
 Operator : SY/MD
 Sample : K6056-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFE08

Manual Integrations
 APPROVED

MMDadoda
 11/27/2019 11:40:31 AM

Quant Time: Nov 27 04:21:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 27 03:09:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	330791	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	325433	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	144033	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	80181	3.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.40%
7) Chloroethane-d5	1.58	69	77284	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.80%
11) 1,1-Dichloroethene-d2	2.13	63	112451	3.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.20%
20) 2-Butanone-d5	3.96	46	263144	61.83	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.66%
24) Chloroform-d	4.40	84	184663	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.08	65	102039	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.10	84	361497	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
36) 1,2-Dichloropropane-d6	6.11	67	117592	4.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.00%
41) Toluene-d8	7.36	98	295318	3.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.00%
43) trans-1,3-Dichloropropene-	7.66	79	40841	4.19	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.80%
46) 2-Hexanone-d5	8.14	63	187180	52.11	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.22%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	93651	5.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	128327	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%

Target Compounds				Ovalue
13) Acetone	2.22	43	10397m	3.493 ug/L

7m2
 11/27/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed