

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112619\
 Data File : VV013802.D
 Acq On : 26 Nov 2019 21:39
 Operator : SY/MD
 Sample : K6056-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFE09

Manual Integrations
 APPROVED

MMDadoda
 11/27/2019 11:40:35 AM

Quant Time: Nov 27 04:27:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 27 03:09:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	345313	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	351985	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	150678	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	80583	3.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.40%
7) Chloroethane-d5	1.58	69	78632	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.60%
11) 1,1-Dichloroethene-d2	2.13	63	110104	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	3.92	46	244546	55.04	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.08%
24) Chloroform-d	4.40	84	177633	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
26) 1,2-Dichloroethane-d4	5.08	65	99371	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.10	84	353720	3.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.00%
36) 1,2-Dichloropropane-d6	6.11	67	115147	4.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.00%
41) Toluene-d8	7.36	98	290896	3.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.20%#
43) trans-1,3-Dichloropropene-	7.66	79	38424	3.65	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.00%
46) 2-Hexanone-d5	8.13	63	171835	44.23	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.46%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	87683	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	127788	4.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.00%

Target Compounds				Ovalue
13) Acetone	2.18	43	12392m	3.988 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112619\
Data File : VV013802.D
Acq On : 26 Nov 2019 21:39
Operator : SY/MD
Sample : K6056-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BFE09

Manual Integrations
APPROVED

MMDadoda
11/27/2019 11:40:35 AM

Quant Time: Nov 27 04:27:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 27 03:09:16 2019
Response via : Initial Calibration

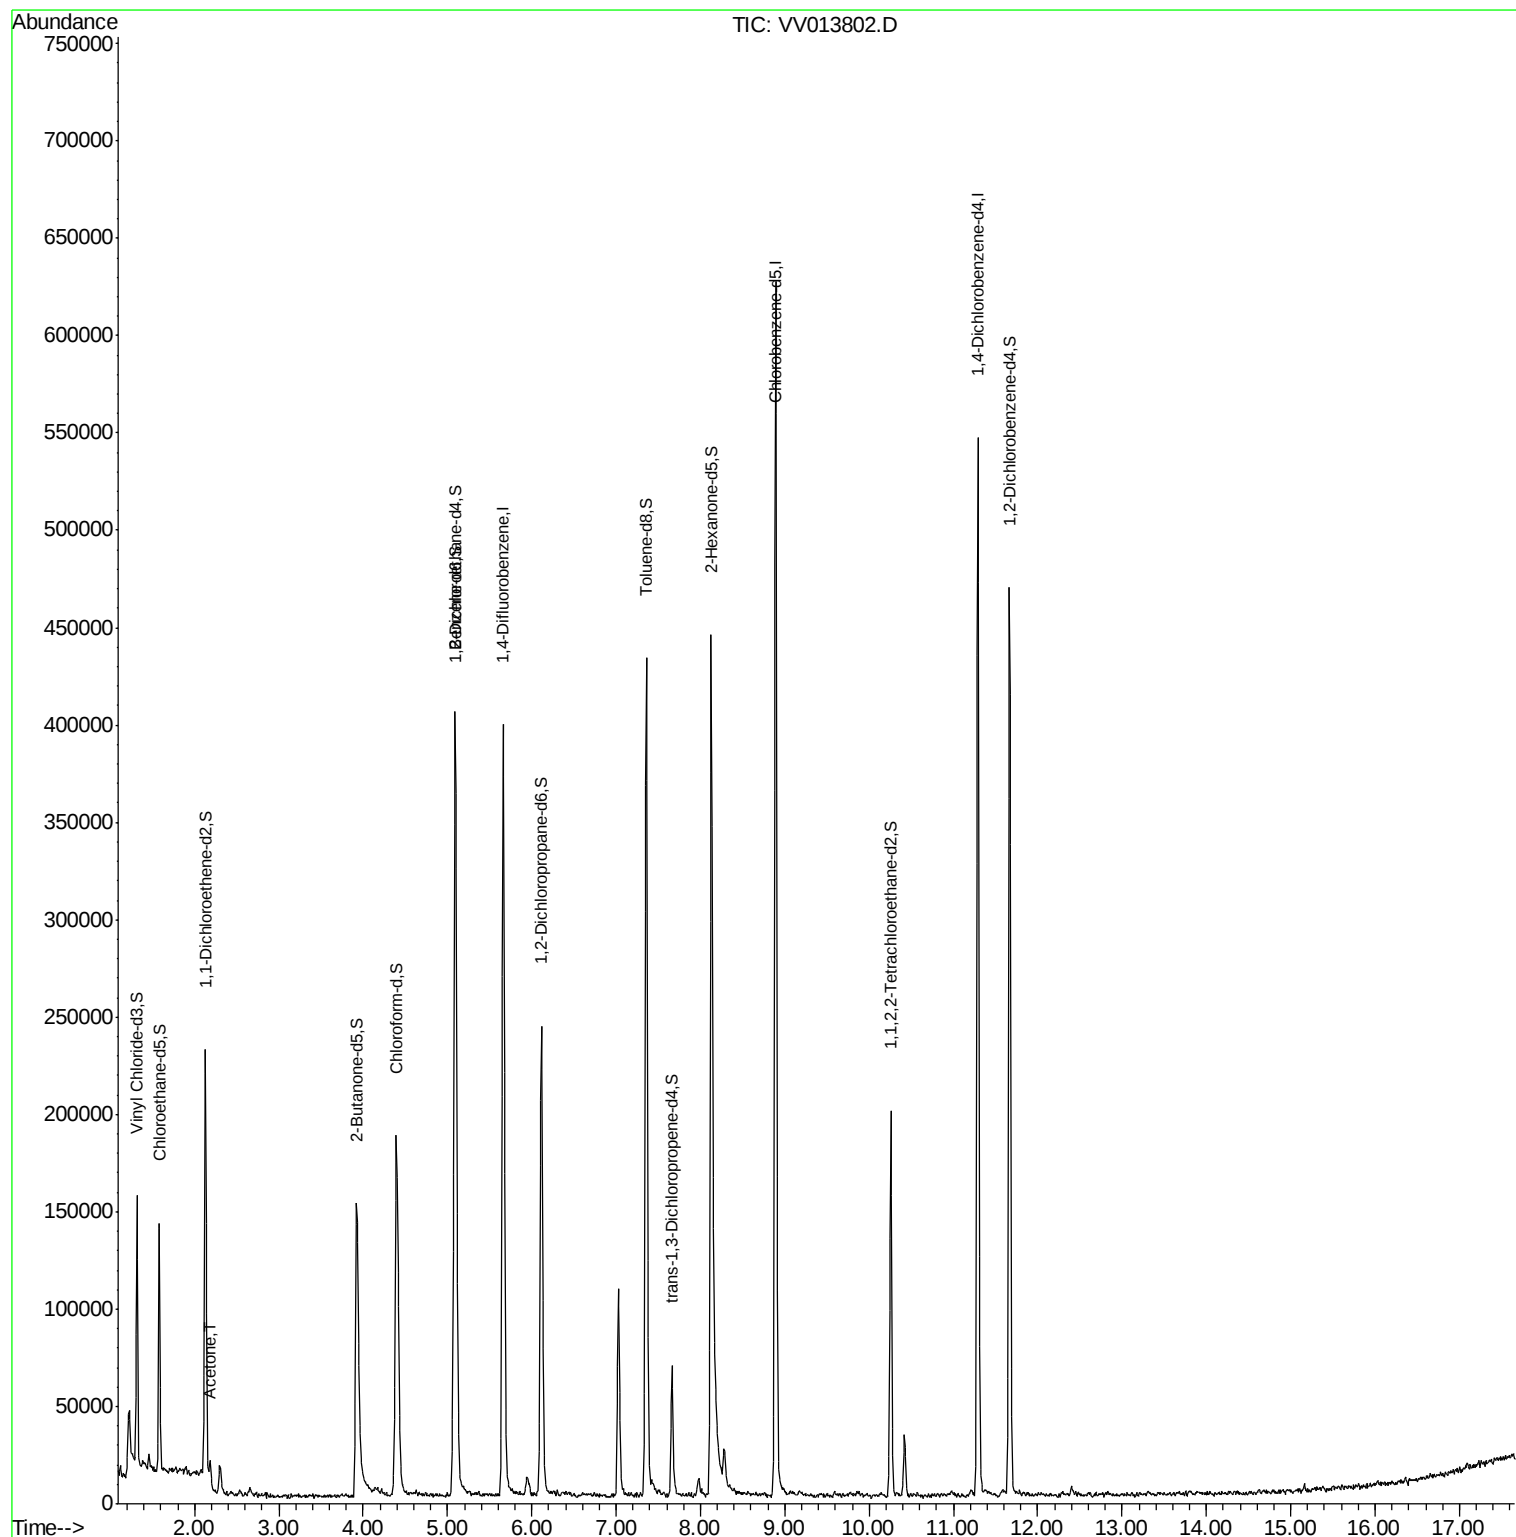

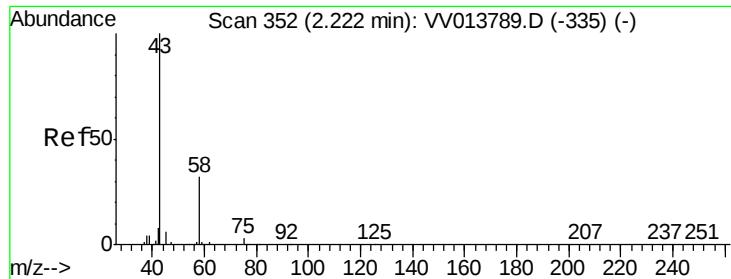

#13

Acetone

Concen: 3.988 ug/L m

RT: 2.18 min Scan# 340

Delta R.T. -0.04 min

Lab File: VV013802.D

Acq: 26 Nov 2019 21:39

Instrument :
MSVOA_V
ClientSampleId :
BFE09

Tot Ion	Ratio	Lower	Upper
43	100		
58	1.5	0.0	27.2

Manual Integrations
APPROVED

MMDadoda
11/27/2019 11:40:35 AM

