

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112619\
 Data File : VV013795.D
 Acq On : 26 Nov 2019 18:51
 Operator : SY/MD
 Sample : K6003-02DL 20X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AE3DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.132	9	13	21	rVB	21359	23291	1.47%	0.214%
2	1.315	62	70	79	rBV2	154937	167992	10.64%	1.546%
3	1.579	146	152	160	rVB	130108	139442	8.83%	1.284%
4	2.126	313	322	341	rVB3	268942	428199	27.11%	3.942%
5	3.225	654	664	681	rVB	33393	71552	4.53%	0.659%
6	3.958	876	892	945	rBV2	533714	1579517	100.00%	14.540%
7	4.396	1010	1028	1051	rBV	194856	492238	31.16%	4.531%
8	5.090	1224	1244	1269	rBV2	418349	1032053	65.34%	9.500%
9	5.659	1407	1421	1446	rBV	384576	774234	49.02%	7.127%
10	5.955	1499	1513	1530	rBV	292924	578393	36.62%	5.324%
11	6.113	1547	1562	1586	rBV	243687	502229	31.80%	4.623%
12	7.029	1835	1847	1866	rBV2	113536	208984	13.23%	1.924%
13	7.357	1935	1949	1965	rBV	424030	739731	46.83%	6.809%
14	7.663	2032	2044	2057	rBV	68104	116627	7.38%	1.074%
15	8.019	2147	2155	2163	rVB	8689	17192	1.09%	0.158%
16	8.138	2178	2192	2225	rBV3	467993	1111670	70.38%	10.233%
17	8.891	2412	2426	2445	rBV	588029	977300	61.87%	8.996%
18	10.257	2839	2851	2866	rBV	208576	327379	20.73%	3.014%
19	10.421	2894	2902	2913	rVB3	15818	27163	1.72%	0.250%
20	11.289	3160	3172	3189	rBV	504233	804951	50.96%	7.410%
21	11.666	3275	3289	3308	rBV	465806	743241	47.05%	6.842%


Sum of corrected areas: 10863378

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112619\
Data File : VV013795.D
Acq On : 26 Nov 2019 18:51
Operator : SY/MD
Sample : K6003-02DL 20X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AE3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

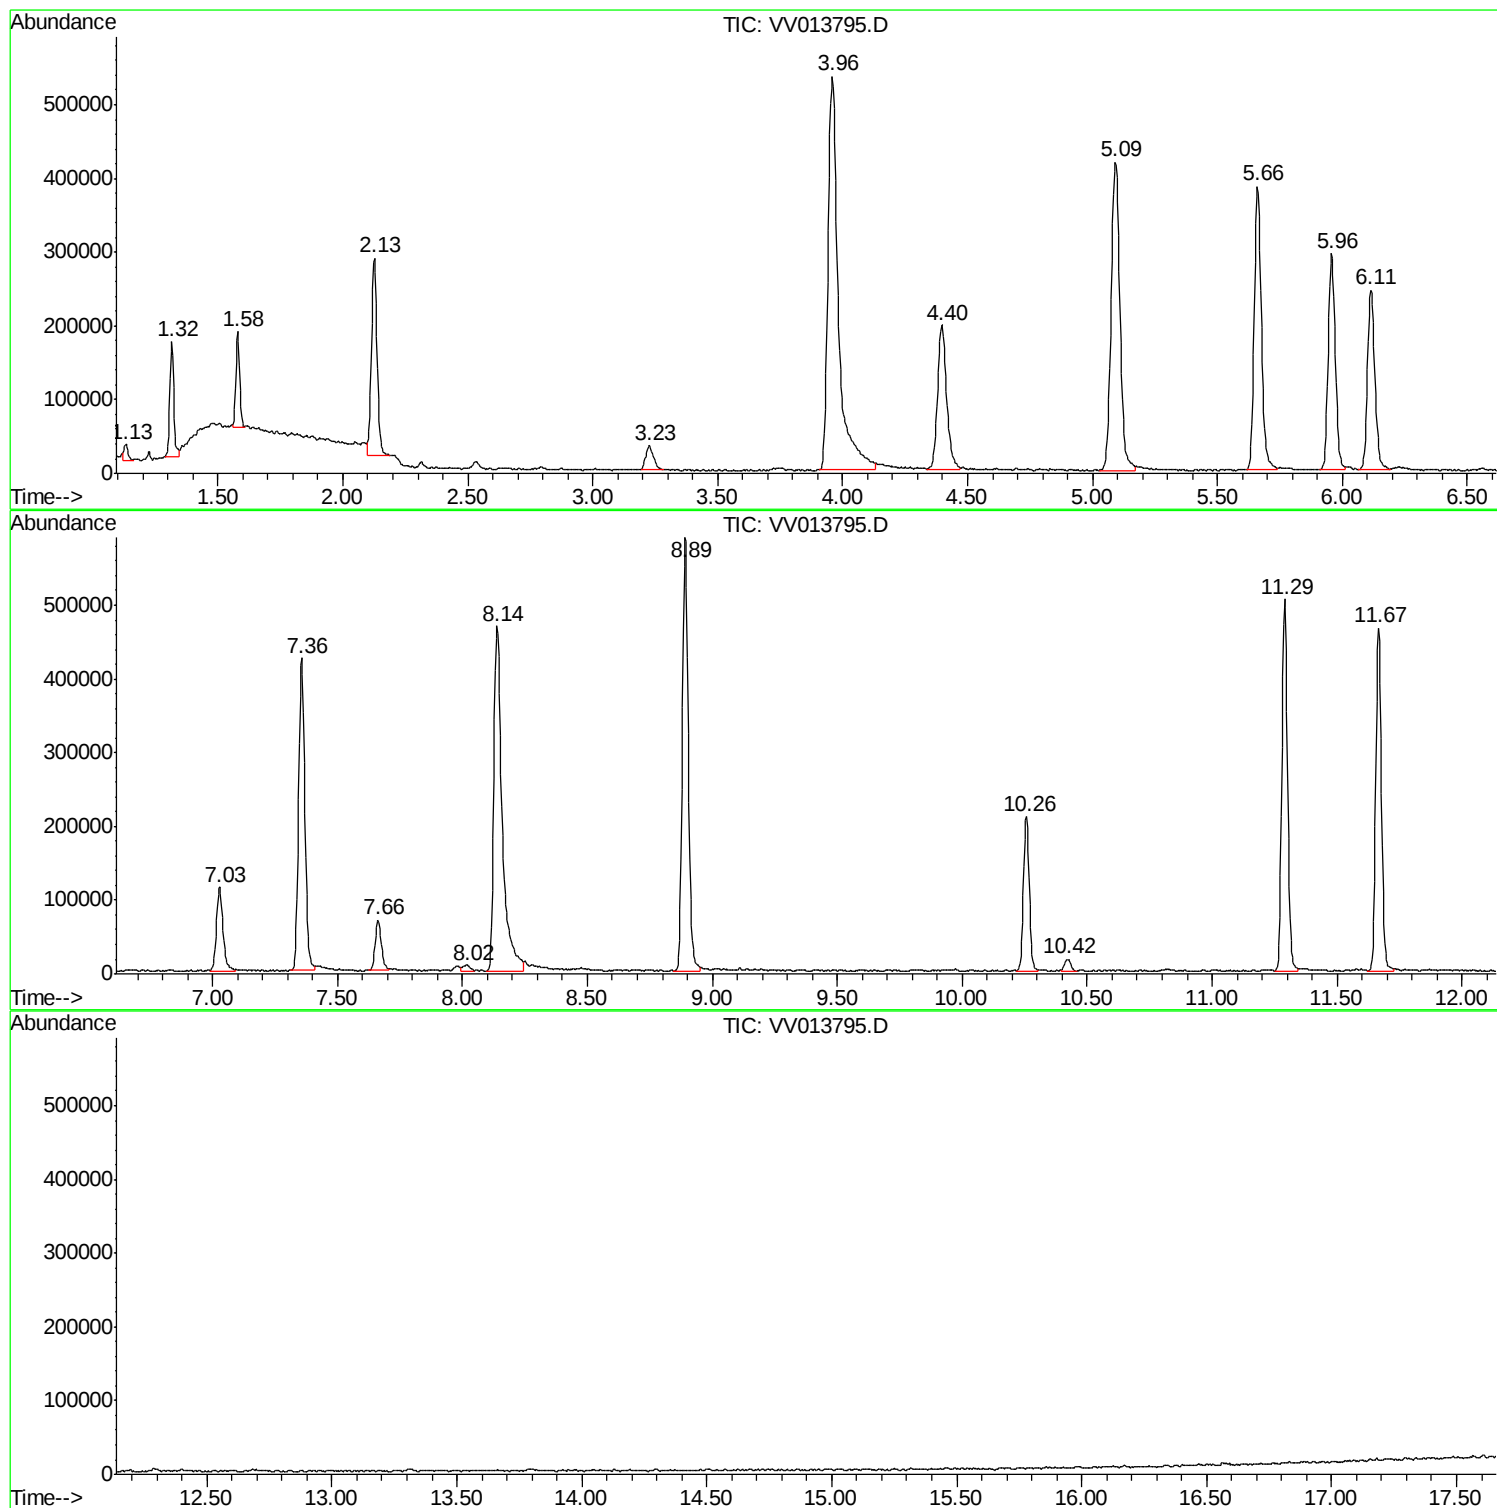

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112619\
Data File : VV013795.D
Acq On : 26 Nov 2019 18:51
Operator : SY/MD
Sample : K6003-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AE3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112619\
Data File : VV013795.D
Acq On : 26 Nov 2019 18:51
Operator : SY/MD
Sample : K6003-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AE3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc