


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112619\
 Data File : VV013776.D
 Acq On : 26 Nov 2019 09:15
 Operator : SY/MD
 Sample : BFB39
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB39

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Nov 28 02:51:59 2019

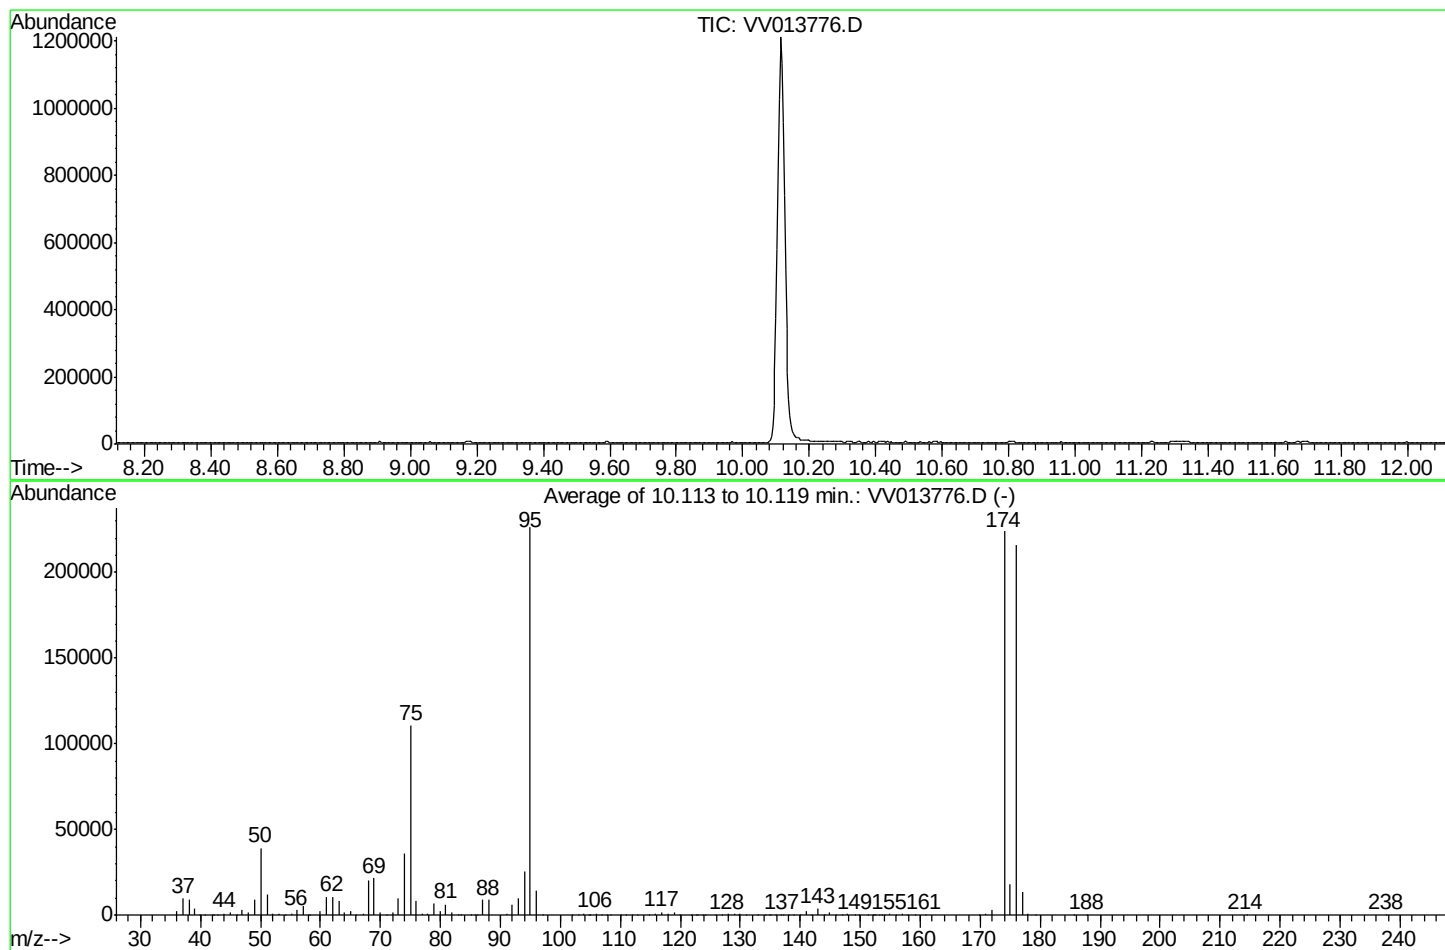

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	39077	PASS
75	95	30	80	48.7	110338	PASS
95	95	100	100	100.0	226346	PASS
96	95	5	9	6.4	14487	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	99.1	224234	PASS
175	174	5	9	7.9	17688	PASS
176	174	95	101	96.2	215701	PASS
177	176	5	9	6.1	13192	PASS

m/z	Abundance
36.00	2140.0
37.10	9695.0
38.10	9402.0
39.00	3935.0
39.90	1085.0
40.70	276.0
42.20	210.0
42.90	307.0
44.00	1567.0
45.10	1802.0
46.00	320.0
47.00	2723.0
48.00	1511.0
49.00	8877.0
50.10	40208.0
51.10	12597.0
52.10	831.0
53.10	359.0
54.10	211.0
55.20	471.0
56.00	3162.0
57.10	5298.0
58.20	366.0
59.10	177.0
60.00	2046.0
61.00	10708.0
62.10	10400.0
63.10	8810.0
64.00	1412.0
65.00	2068.0
66.00	465.0
67.10	820.0
68.00	20320.0
69.00	21832.0
70.00	1739.0
71.00	209.0
72.10	1187.0
73.00	9464.0
74.00	36600.0
75.10	112360.0
76.00	8338.0
77.00	1332.0
77.90	959.0
79.00	6611.0
80.00	2090.0
80.90	6607.0
81.90	1232.0
83.00	140.0
83.30	148.0
85.10	156.0
85.80	322.0
86.20	347.0
87.00	8988.0
88.00	9075.0
89.60	116.0
91.00	773.0
92.00	5883.0
93.00	9720.0
94.00	26200.0
95.00	229440.0
96.00	14822.0
97.00	338.0
103.10	172.0
103.90	774.0
104.80	351.0
105.90	836.0
106.80	228.0
107.80	176.0
108.40	119.0
110.00	188.0
110.90	177.0
111.90	300.0
112.80	368.0
114.90	330.0
115.90	853.0
116.90	1553.0
117.90	726.0
118.90	1369.0
122.70	120.0
123.80	123.0
124.20	156.0
125.90	209.0
126.90	105.0
128.00	730.0
129.00	459.0
129.70	539.0
131.00	323.0
132.90	125.0
134.90	359.0
136.00	103.0
136.80	284.0
137.20	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

138.10	106.0
138.80	156.0
141.00	1942.0
141.80	415.0
143.00	3755.0
143.90	302.0
144.90	1451.0
146.00	421.0
146.90	342.0
147.80	662.0
149.10	156.0
149.80	303.0
152.30	167.0
153.10	188.0
154.00	308.0
155.00	735.0
155.90	165.0
156.90	576.0
157.90	118.0
159.00	295.0
160.90	293.0
170.90	1064.0
172.00	3133.0
174.00	220416.0
175.00	17872.0
176.00	210432.0
177.00	13283.0
177.90	551.0
179.30	109.0
207.00	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	2305.0
37.10	9607.0
38.10	9696.0
39.00	4039.0
39.90	1057.0
40.70	353.0
42.20	216.0
42.90	258.0
44.00	1635.0
45.00	1824.0
46.10	342.0
47.00	2953.0
48.00	1464.0
49.00	9107.0
50.10	40344.0
51.10	12386.0
52.10	884.0
53.10	416.0
54.10	265.0
55.20	751.0
56.00	2905.0
57.10	5659.0
58.10	314.0
59.10	164.0
60.00	2146.0
61.00	11077.0
62.10	11225.0
63.10	8669.0
64.00	1457.0
65.00	1991.0
66.00	407.0
67.10	738.0
68.10	21024.0
69.00	22168.0
70.10	1653.0
71.00	209.0
72.00	1227.0
73.00	9832.0
74.00	37352.0
75.10	113752.0
76.00	8930.0
77.00	1101.0
77.90	1007.0
79.00	7098.0
80.00	2241.0
80.90	6412.0
81.90	1311.0
83.00	163.0
85.10	154.0
87.00	8959.0
88.00	9020.0
91.00	697.0
92.00	6256.0
93.00	10422.0
94.00	26776.0
95.00	233792.0
96.00	15024.0
97.00	362.0
101.90	139.0
103.90	777.0
104.80	338.0
106.00	888.0
106.80	243.0
107.80	211.0
110.00	208.0
110.90	256.0
111.90	321.0
112.80	354.0
114.90	407.0
115.90	945.0
116.90	1619.0
117.90	883.0
119.00	1433.0
119.80	110.0
122.90	103.0
123.70	153.0
124.30	158.0
125.90	192.0
127.00	126.0
127.90	758.0
128.90	439.0
129.90	565.0
130.90	332.0
132.90	181.0
135.10	371.0
136.00	121.0
136.80	241.0
137.20	311.0
138.80	131.0
139.90	143.0
141.00	1911.0
141.80	381.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

143.00	3800.0
143.90	301.0
144.90	1496.0
145.90	415.0
147.00	322.0
147.90	703.0
149.10	203.0
149.80	295.0
152.50	126.0
153.10	170.0
154.10	262.0
155.00	753.0
156.00	137.0
157.00	576.0
157.90	102.0
159.00	291.0
160.90	308.0
169.80	122.0
170.90	987.0
172.00	3264.0
174.00	231936.0
175.00	18360.0
176.00	223360.0
177.00	13598.0
177.90	531.0
185.70	102.0
187.80	114.0
207.00	145.0
237.70	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	2237.0
37.10	8922.0
38.10	9003.0
39.00	3725.0
39.90	924.0
40.70	330.0
41.30	109.0
41.90	180.0
42.30	183.0
42.90	202.0
44.00	1715.0
45.00	1644.0
46.10	306.0
47.00	2867.0
48.00	1326.0
49.00	8194.0
50.10	36680.0
51.10	11179.0
52.10	773.0
53.00	453.0
54.10	288.0
55.20	809.0
56.00	2636.0
57.10	5292.0
57.90	325.0
60.00	2022.0
61.00	10141.0
62.00	10435.0
63.10	7740.0
64.10	1323.0
65.10	1753.0
66.00	322.0
67.10	592.0
68.10	19656.0
69.00	20448.0
70.10	1356.0
71.00	196.0
72.10	1224.0
73.00	9205.0
74.00	33496.0
75.10	104904.0
76.00	8748.0
77.10	935.0
78.00	989.0
79.00	6611.0
80.00	2164.0
80.90	5837.0
81.90	1237.0
83.10	170.0
85.00	166.0
87.00	8156.0
88.00	8426.0
91.10	647.0
92.00	5895.0
93.00	9796.0
94.00	24384.0
95.00	215808.0
96.00	13615.0
97.00	301.0
103.90	754.0
105.00	327.0
106.00	902.0
106.80	252.0
107.80	209.0
110.10	198.0
110.90	307.0
111.90	279.0
112.90	263.0
114.80	385.0
115.90	992.0
116.90	1482.0
117.90	1013.0
119.00	1386.0
119.80	104.0
121.80	100.0
122.90	107.0
123.70	167.0
125.90	108.0
127.10	183.0
127.80	745.0
128.90	414.0
130.00	676.0
130.80	326.0
132.90	160.0
134.10	105.0
135.00	329.0
135.80	144.0
136.80	230.0
137.10	259.0
139.80	140.0
140.90	1853.0
141.80	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

143.00	3327.0
144.00	253.0
144.90	1390.0
146.00	363.0
147.10	260.0
147.90	595.0
149.20	223.0
149.80	220.0
151.20	105.0
152.00	114.0
153.10	159.0
153.70	114.0
154.20	221.0
154.90	727.0
155.90	132.0
157.00	569.0
159.10	334.0
160.80	253.0
169.80	173.0
170.90	834.0
172.00	3109.0
174.00	220352.0
175.00	16832.0
176.00	213312.0
177.00	12695.0
177.90	429.0
185.70	106.0
187.80	104.0
207.00	175.0
214.30	102.0
237.70	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.20	160.0
37.60	187.0
40.00	842.0
41.20	162.0
42.20	182.0
42.80	128.0
44.00	882.0
45.00	149.0
45.30	155.0
46.70	158.0
51.50	161.0
57.30	136.0
59.00	144.0
60.00	132.0
68.80	107.0
76.10	114.0
89.50	133.0
149.40	126.0
153.30	111.0
191.30	151.0
207.00	155.0
235.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39