

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW112621\  
 Data File : VW023721.D  
 Acq On : 26 Nov 2021 13:25  
 Operator : SY/MD  
 Sample : M4821-20  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :

Quant Time: Nov 27 03:52:54 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Nov 27 03:48:32 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.616  | 114   | 134351   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.853  | 117   | 128726   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152   | 68147    | 5.000    | ug/L   | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.304  | 65    | 42149    | 3.822    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 76.400%  |
| 7) Chloroethane-d5            | 1.564  | 69    | 37069    | 4.276    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 85.600%  |
| 11) 1,1-Dichloroethene-d2     | 2.105  | 63    | 62333    | 3.207    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 64.200%  |
| 20) 2-Butanone-d5             | 3.937  | 46    | 61090    | 46.075   | ug/L   | 0.04     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 92.160%  |
| 24) Chloroform-d              | 4.349  | 84    | 87881    | 4.576    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 91.600%  |
| 26) 1,2-Dichloroethane-d4     | 5.034  | 65    | 39824    | 4.439    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 88.800%  |
| 32) Benzene-d6                | 5.050  | 84    | 170182   | 4.853    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 97.000%  |
| 36) 1,2-Dichloropropane-d6    | 6.069  | 67    | 48301    | 4.913    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 98.200%  |
| 41) Toluene-d8                | 7.317  | 98    | 153931   | 4.698    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 94.000%  |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79    | 17764    | 4.483    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 89.600%  |
| 46) 2-Hexanone-d5             | 8.095  | 63    | 58685    | 44.575   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 89.140%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84    | 32580    | 4.606    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 92.200%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.625 | 152   | 62314    | 5.172    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 103.400% |
| Target Compounds              |        |       |          |          |        |          |
|                               |        |       |          |          | Qvalue |          |
| 5) Vinyl chloride             | 1.310  | 62    | 31124    | 2.674    | ug/L   | 96       |
| 8) Chloroethane               | 1.580  | 64    | 2835     | 0.384    | ug/L   | 90       |
| 12) 1,1-Dichloroethene        | 2.101  | 96    | 764      | 0.085    | ug/L # | 1        |
| 13) Acetone                   | 2.224  | 43    | 9323     | 7.814    | ug/L   | 75       |
| 14) Carbon disulfide          | 2.288  | 76    | 27218    | 0.900    | ug/L   | 100      |
| 15) Methyl Acetate            | 2.429  | 43    | 1727     | 0.638    | ug/L # | 50       |
| 16) Methylene chloride        | 2.503  | 84    | 7799     | 0.607    | ug/L   | 96       |
| 18) trans-1,2-Dichloroethene  | 2.757  | 96    | 7564     | 0.738    | ug/L   | 90       |
| 19) 1,1-Dichloroethane        | 3.188  | 63    | 22326    | 1.295    | ug/L   | 99       |
| 22) cis-1,2-Dichloroethene    | 3.912  | 96    | 58502    | 5.950    | ug/L   | 98       |
| 25) Chloroform                | 4.378  | 83    | 12980    | 0.676    | ug/L   | 100      |
| 33) Benzene                   | 5.101  | 78    | 69292    | 1.888    | ug/L   | 100      |
| 34) Trichloroethene           | 5.918  | 95    | 2177     | 0.221    | ug/L   | 94       |
| 35) Methylcyclohexane         | 6.072  | 83    | 12636    | 0.824    | ug/L # | 19       |
| 37) 1,2-Dichloropropane       | 6.072  | 63    | 6286     | 0.721    | ug/L # | 84       |
| 39) cis-1,3-Dichloropropene   | 6.989  | 75    | 1356     | 0.109    | ug/L # | 70       |
| 42) Toluene                   | 7.387  | 91    | 126140   | 3.169    | ug/L   | 97       |
| 45) 1,1,2-Trichloroethane     | 7.709  | 97    | 1078     | 0.178    | ug/L # | 16       |
| 51) Chlorobenzene             | 8.882  | 112   | 4587     | 0.174    | ug/L   | 95       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112621\  
 Data File : VV023721.D  
 Acq On : 26 Nov 2021 13:25  
 Operator : SY/MD  
 Sample : M4821-20  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :

Quant Time: Nov 27 03:52:54 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Nov 27 03:48:32 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|-------|--------|----------|
| 52) Ethylbenzene              | 9.011  | 91   | 101480   | 2.439 | ug/L   | 100      |
| 53) m,p-xylene                | 9.136  | 106  | 72806    | 4.397 | ug/L   | 99       |
| 54) o-xylene                  | 9.542  | 106  | 59575    | 3.783 | ug/L   | 99       |
| 55) Styrene                   | 9.542  | 104  | 3627     | 0.137 | ug/L # | 1        |
| 60) Isopropylbenzene          | 9.931  | 105  | 4435     | 0.109 | ug/L # | 90       |
| 61) 1,2,3-Trichloropropane    | 10.014 | 75   | 743      | 0.154 | ug/L # | 1        |
| 62) 1,3,5-Trimethylbenzene    | 10.541 | 105  | 11929    | 0.352 | ug/L   | 94       |
| 63) 1,2,4-Trimethylbenzene    | 10.914 | 105  | 21568    | 0.644 | ug/L   | 100      |
| 68) 1,2-Dibromo-3-chloropr... | 12.464 | 75   | 156      | 0.163 | ug/L # | 1        |
| 71) Naphthalene               | 13.503 | 128  | 59452    | 3.505 | ug/L   | 99       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112621\  
Data File : VV023721.D  
Acq On : 26 Nov 2021 13:25  
Operator : SY/MD  
Sample : M4821-20  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :


Quant Time: Nov 27 03:52:54 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Nov 27 03:48:32 2021  
Response via : Initial Calibration

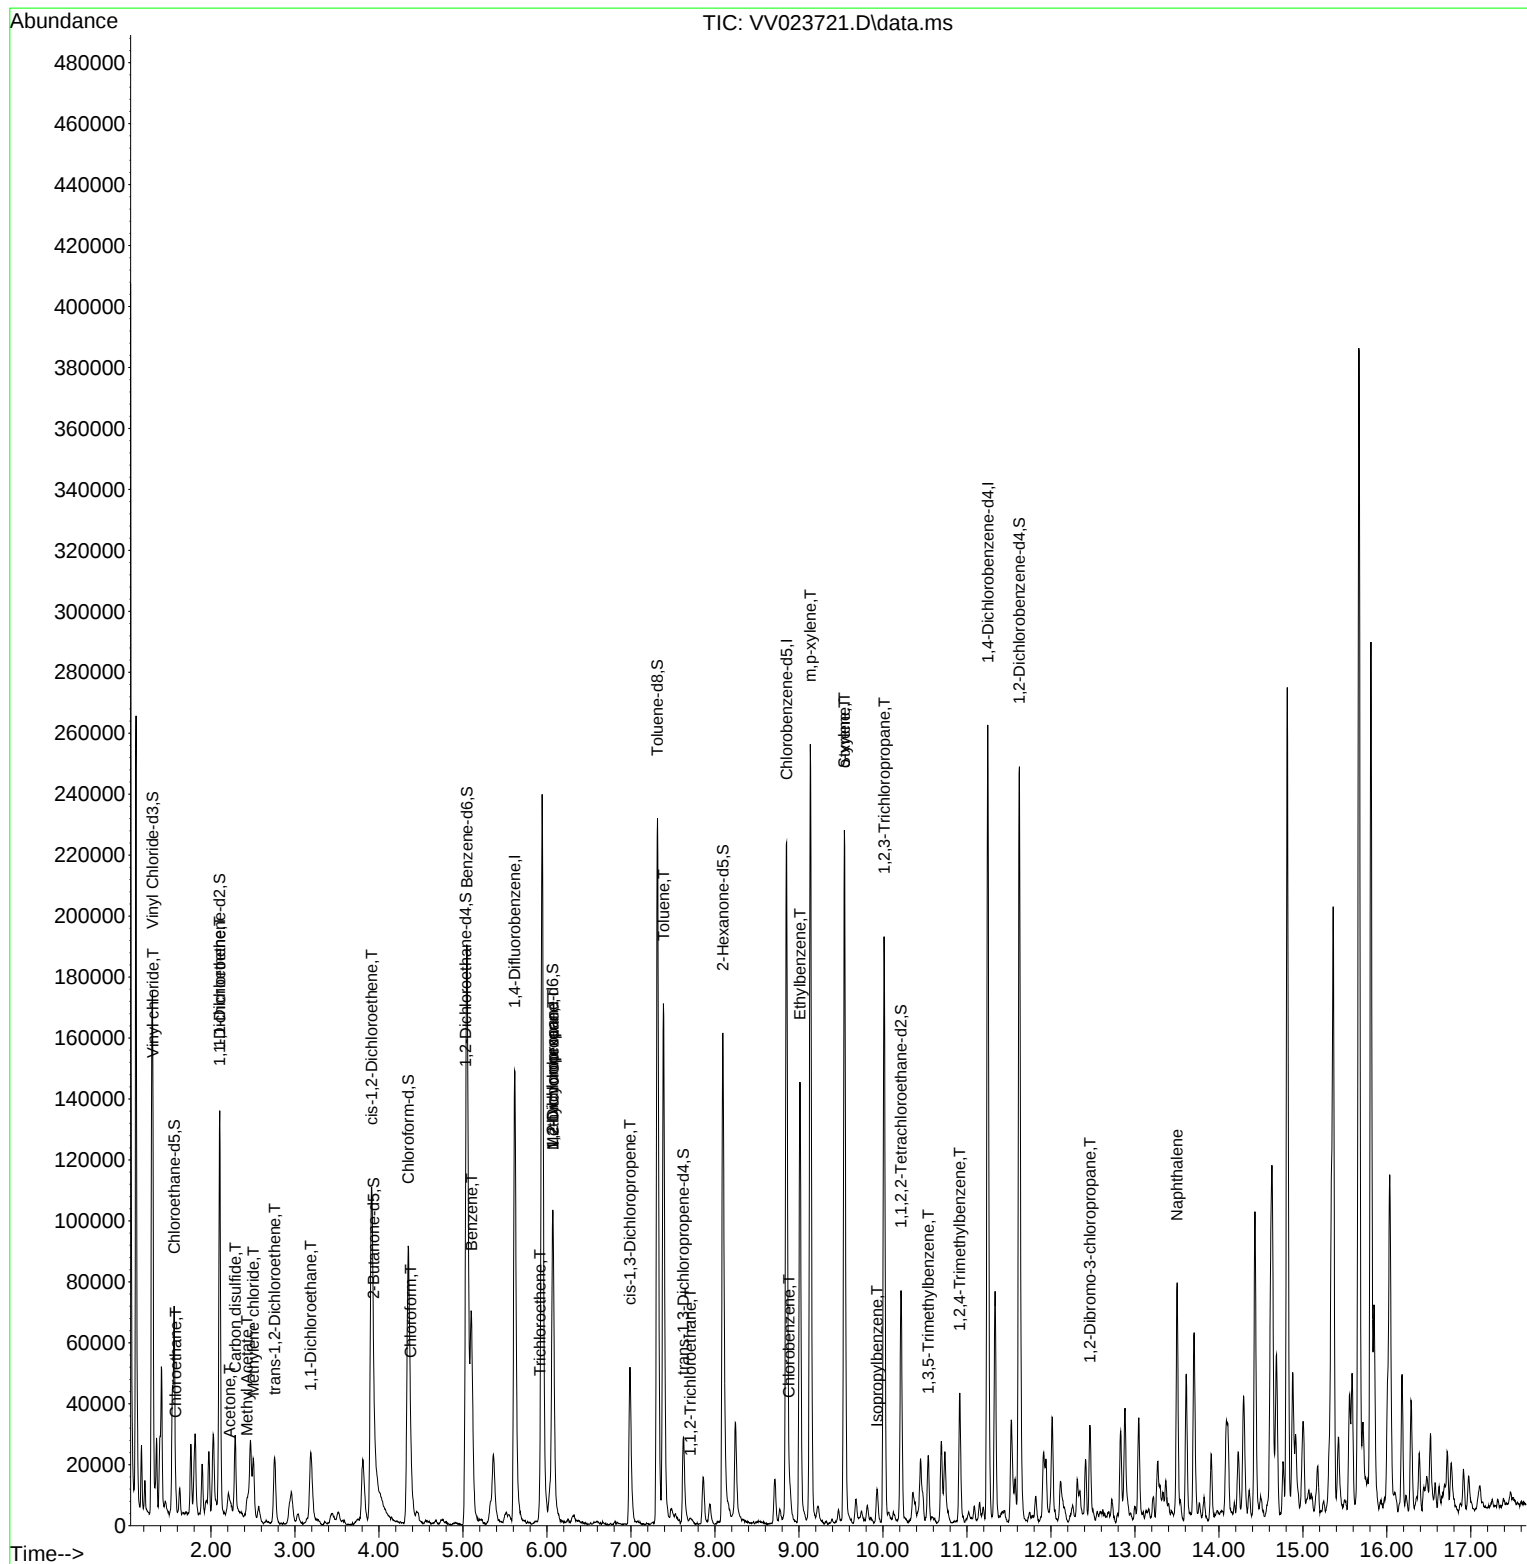



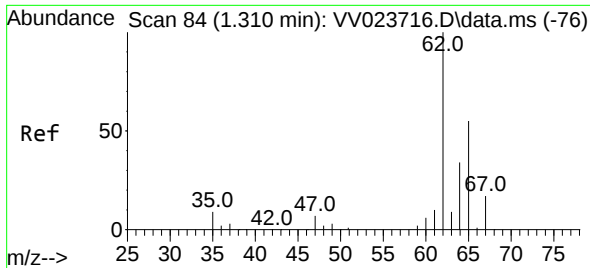


#5  
 Vinyl chloride  
 Concen: 2.674 ug/L  
 RT: 1.310 min Scan# 84  
 Delta R.T. -0.000 min  
 Lab File: VV023721.D  
 Acq: 26 Nov 2021 13:25

Instrument :  
 MSVOA\_V  
 ClientSampleId :



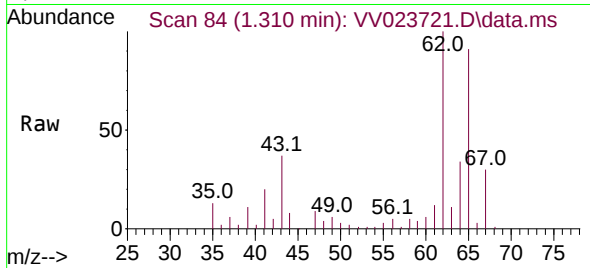



Tgt Ion: 62 Resp: 31124  
 Ion Ratio Lower Upper  
 62 100  
 64 34.2 22.4 41.6

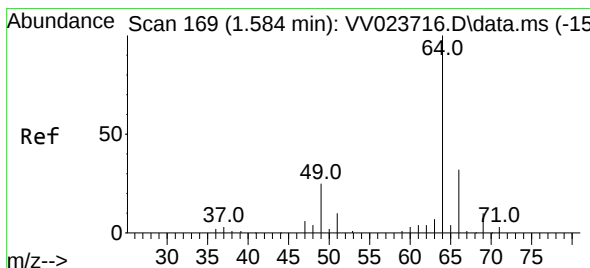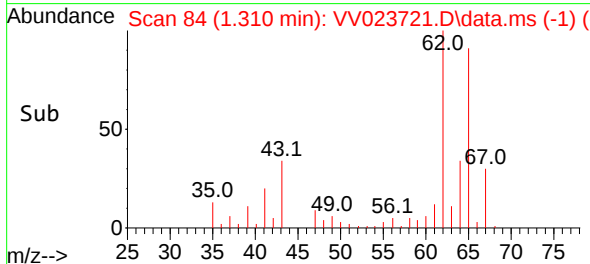

#8  
 Chloroethane  
 Concen: 0.384 ug/L  
 RT: 1.580 min Scan# 168  
 Delta R.T. -0.003 min  
 Lab File: VV023721.D  
 Acq: 26 Nov 2021 13:25

Tgt Ion: 64 Resp: 2835  
 Ion Ratio Lower Upper  
 64 100  
 66 25.1 21.4 39.8

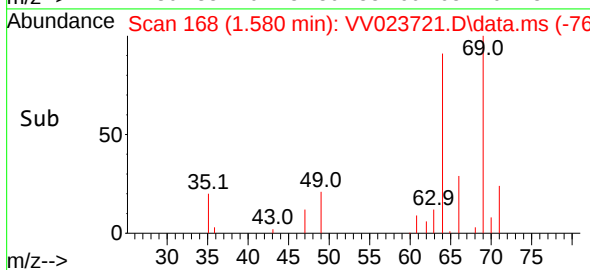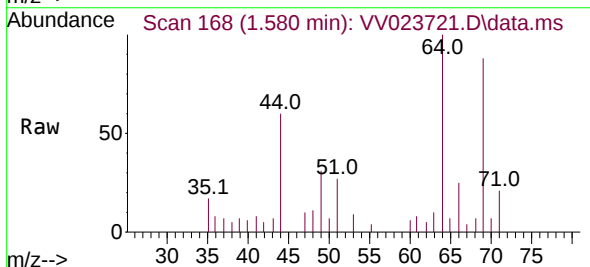



#12

1,1-Dichloroethene

Concen: 0.085 ug/L

RT: 2.101 min Scan# 31

Delta R.T. -0.016 min

Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

Instrument :

MSVOA\_V

ClientSampleId :





Tgt Ion: 96 Resp: 764

Ion Ratio Lower Upper

96 100

61 1185.1 116.1 215.5#

63 8505.4 79.4 147.4#

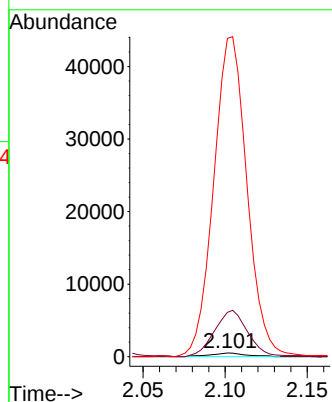

#13

Acetone

Concen: 7.814 ug/L

RT: 2.224 min Scan# 368

Delta R.T. 0.039 min

Lab File: VV023721.D




Acq: 26 Nov 2021 13:25


Tgt Ion: 43 Resp: 9323

Ion Ratio Lower Upper

43 100


58 9.1 0.0 41.4

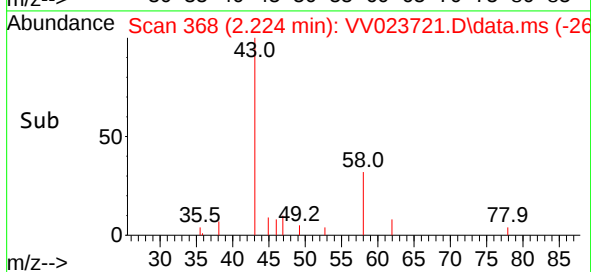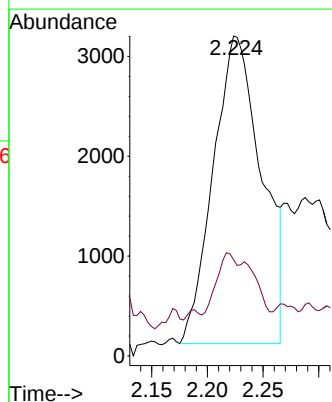






#14  
Carbon disulfide  
Concen: 0.900 ug/L  
RT: 2.288 min Scan# 31  
Delta R.T. -0.006 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25

Instrument :  
MSVOA\_V  
ClientSampleId :







Tgt Ion: 76 Resp: 27218  
Ion Ratio Lower Upper  
76 100  
78 9.2 7.5 11.3

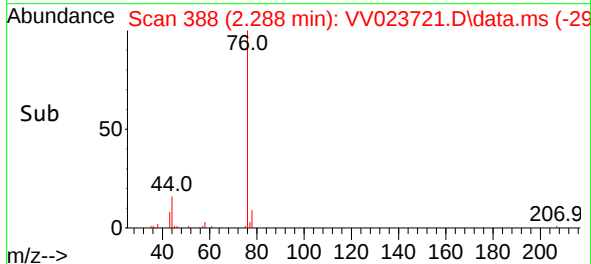

#15  
Methyl Acetate  
Concen: 0.638 ug/L  
RT: 2.429 min Scan# 432  
Delta R.T. -0.010 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25


Tgt Ion: 43 Resp: 1727  
Ion Ratio Lower Upper  
43 100  
74 0.0 20.2 30.2#

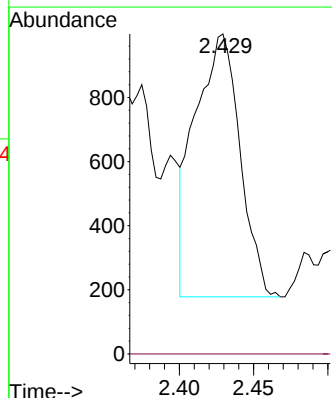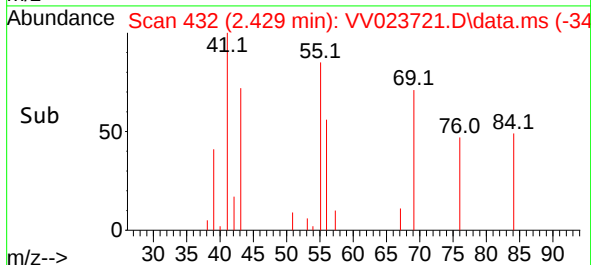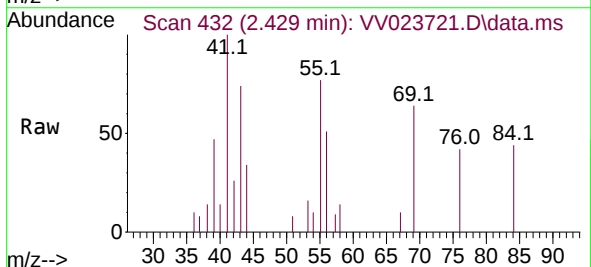






#16  
Methylene chloride  
Concen: 0.607 ug/L  
RT: 2.503 min Scan# 416  
Delta R.T. -0.003 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25

Instrument :  
MSVOA\_V  
ClientSampleId :




Tgt Ion: 84 Resp: 7799

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 86  | 64.5  | 42.6  | 79.0  |
| 49  | 109.2 | 79.7  | 147.9 |

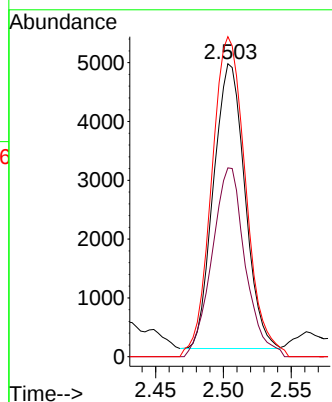




#18  
trans-1,2-Dichloroethene  
Concen: 0.738 ug/L  
RT: 2.757 min Scan# 534  
Delta R.T. -0.000 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25



Tgt Ion: 96 Resp: 7564

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 96  | 100   |       |       |
| 61  | 141.5 | 88.2  | 163.8 |
| 98  | 66.4  | 44.9  | 83.5  |

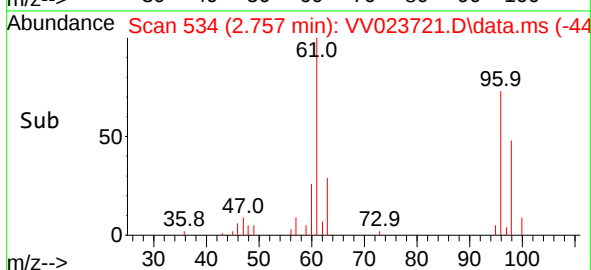



#19

1,1-Dichloroethane

Concen: 1.295 ug/L

RT: 3.188 min Scan# 6

Delta R.T. -0.000 min

Lab File: VV023721.D





Acq: 26 Nov 2021 13:25

Instrument :

MSVOA\_V

ClientSampleId :

|             |             |
|-------------|-------------|
| Tgt Ion: 63 | Resp: 22326 |
| Ion Ratio   | Lower Upper |
| 63 100      |             |
| 65 31.7     | 22.3 41.3   |
| 83 13.8     | 10.7 19.9   |

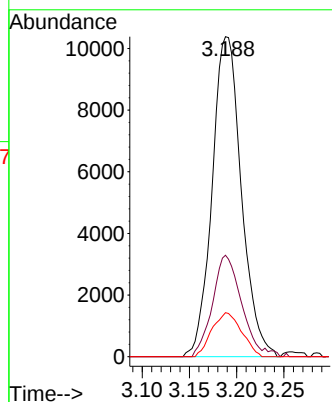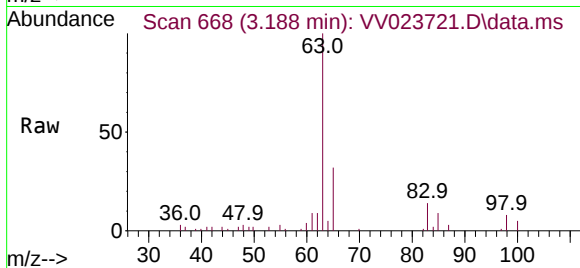

#22

cis-1,2-Dichloroethene

Concen: 5.950 ug/L




RT: 3.912 min Scan# 893


Delta R.T. 0.003 min

Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

|             |             |
|-------------|-------------|
| Tgt Ion: 96 | Resp: 58502 |
| Ion Ratio   | Lower Upper |
| 96 100      |             |
| 61 121.0    | 83.4 154.8  |
| 68 0.0      | 0.0 0.0     |

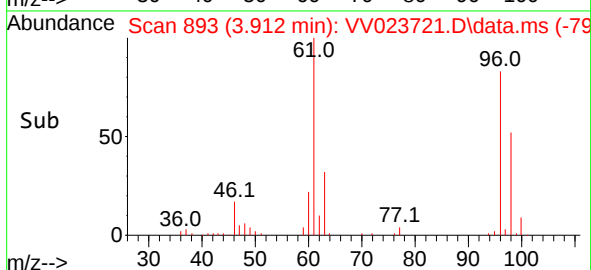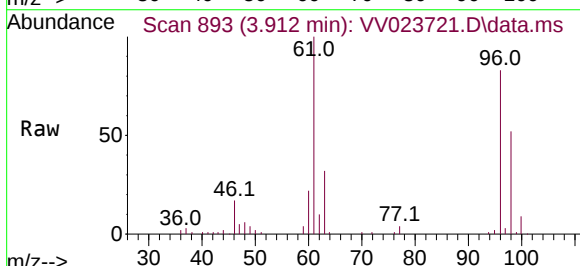

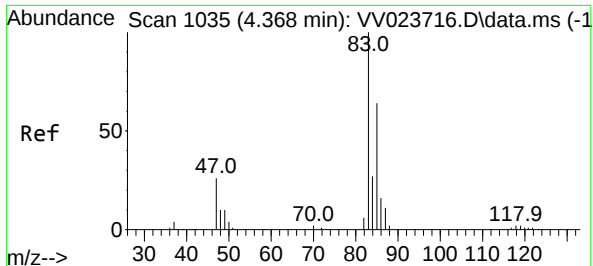

#25

Chloroform

Concen: 0.676 ug/L

RT: 4.378 min Scan# 1035

Delta R.T. 0.010 min

Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

Instrument :

MSVOA\_V





ClientSampleId :

Tgt Ion: 83 Resp: 12980

Ion Ratio Lower Upper

83 100

85 64.8 45.2 84.0

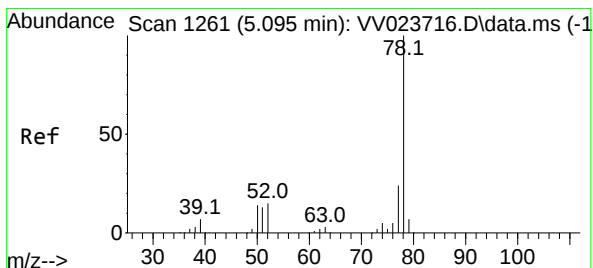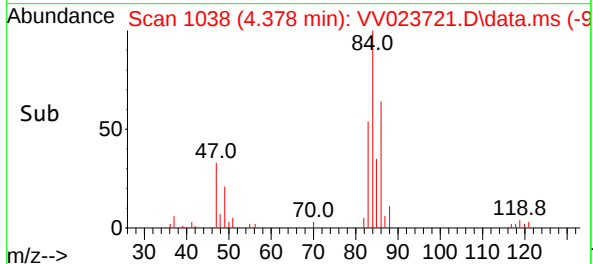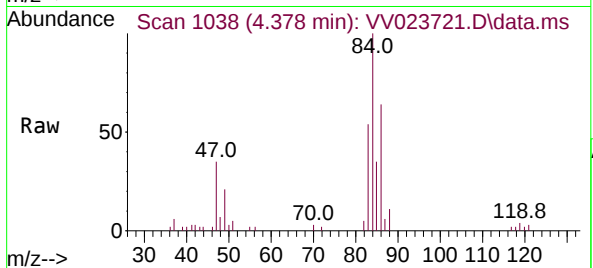

#33

Benzene

Concen: 1.888 ug/L




RT: 5.101 min Scan# 1263


Delta R.T. 0.006 min

Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

Tgt Ion: 78 Resp: 69292


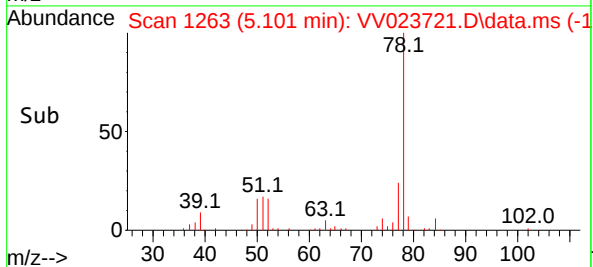

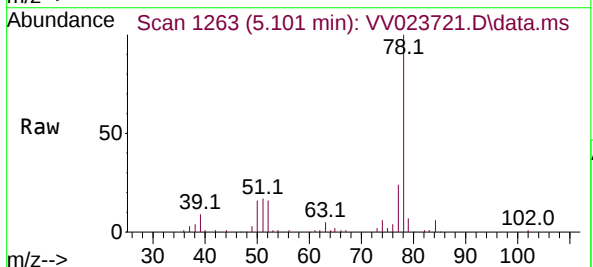


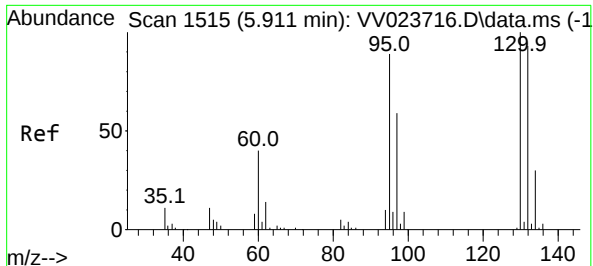

#34  
Trichloroethene  
Concen: 0.221 ug/L  
RT: 5.918 min Scan# 11  
Delta R.T. 0.006 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25




Instrument :  
MSVOA\_V  
ClientSampleId :


Tgt Ion: 95 Resp: 2177  
Ion Ratio Lower Upper  
95 100  
97 74.7 45.2 84.0  
132 115.4 76.1 141.3  
130 109.5 75.4 140.0

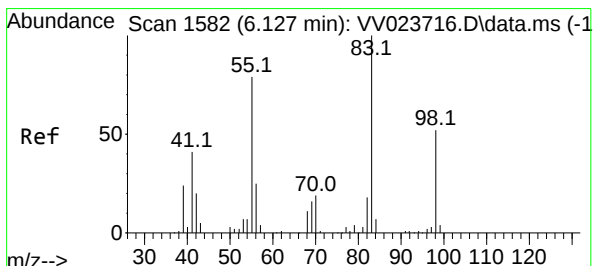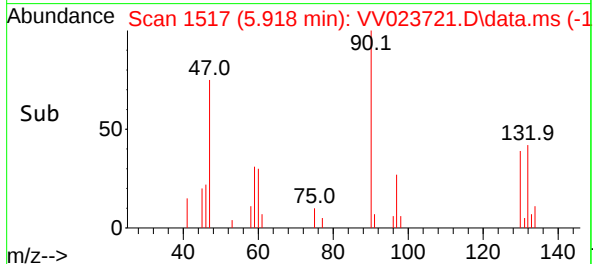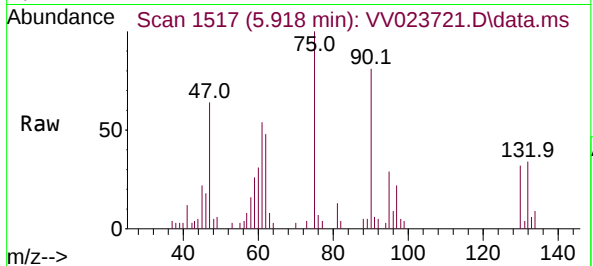

#35  
Methylcyclohexane  
Concen: 0.824 ug/L  
RT: 6.072 min Scan# 1565  
Delta R.T. -0.055 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25

Tgt Ion: 83 Resp: 12636  
Ion Ratio Lower Upper  
83 100  
55 0.7 60.2 90.2#  
98 1.0 41.0 61.4#

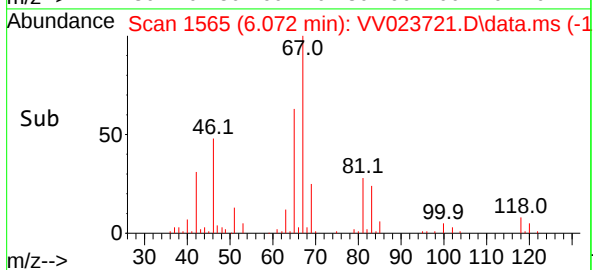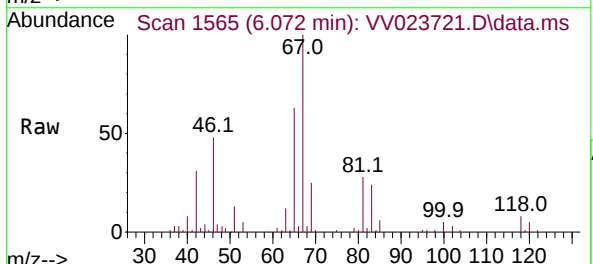

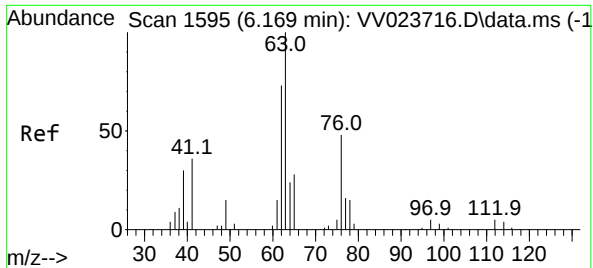

#37

1,2-Dichloropropane

Concen: 0.721 ug/L

RT: 6.072 min Scan# 11

Delta R.T. -0.096 min

Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

Instrument :

MSVOA\_V





ClientSampleId :

Tgt Ion: 63 Resp: 6286

Ion Ratio Lower Upper

63 100

112 0.0 4.3 6.5#

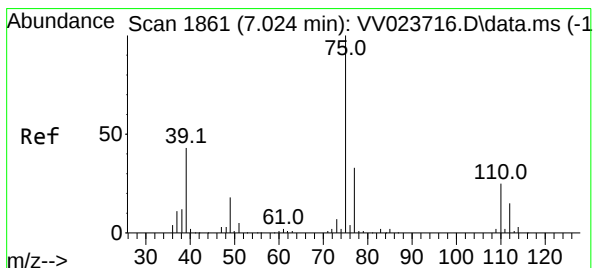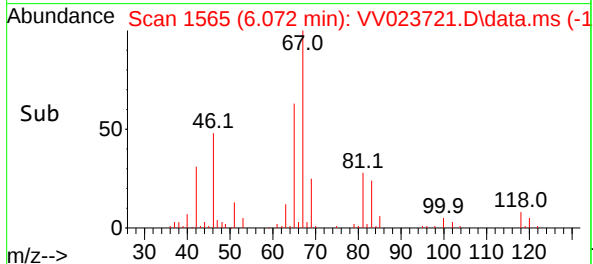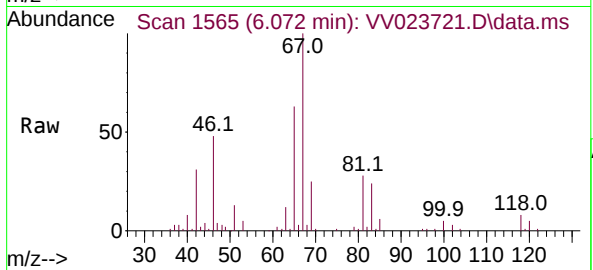

#39

cis-1,3-Dichloropropene

Concen: 0.109 ug/L

RT: 6.989 min Scan# 1850

Delta R.T. -0.035 min

Lab File: VV023721.D




Acq: 26 Nov 2021 13:25


Tgt Ion: 75 Resp: 1356

Ion Ratio Lower Upper

75 100

77 47.9 22.0 41.0#

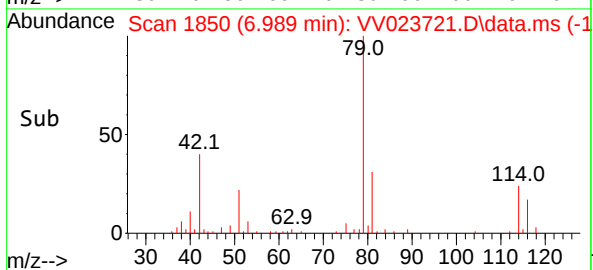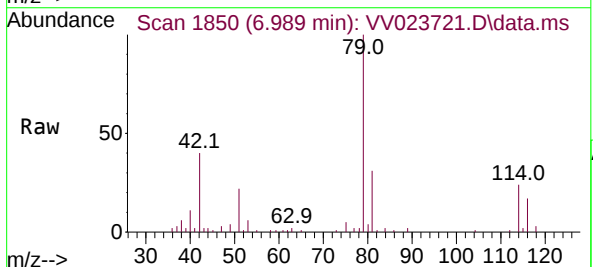

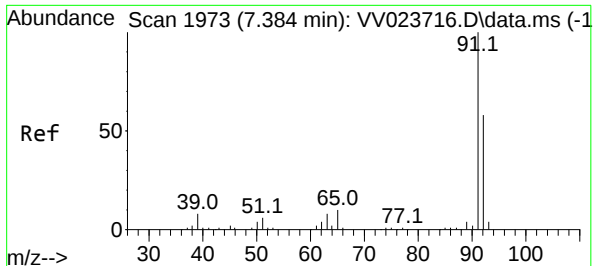

#42

Toluene

Concen: 3.169 ug/L

RT: 7.387 min Scan# 1973

Delta R.T. 0.003 min

Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

Instrument :

MSVOA\_V





ClientSampleId :

Tgt Ion: 91 Resp: 126140

Ion Ratio Lower Upper

91 100

92 56.9 41.5 77.1

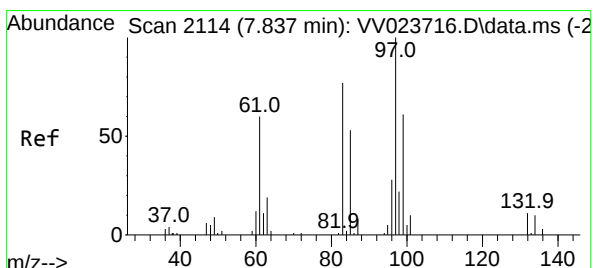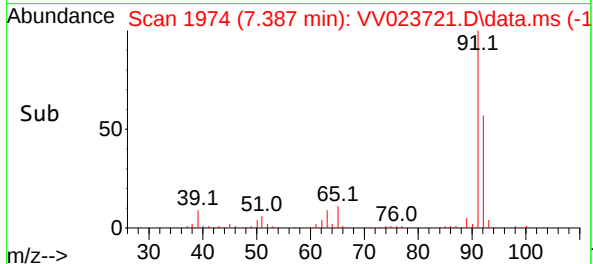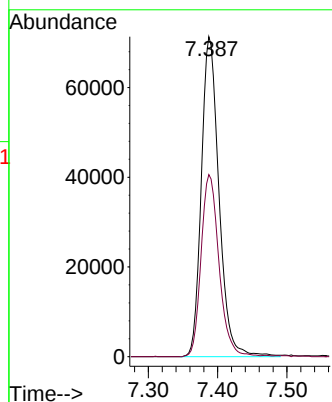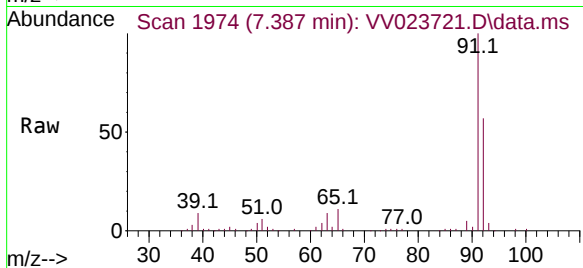

#45

1,1,2-Trichloroethane

Concen: 0.178 ug/L

RT: 7.709 min Scan# 2074

Delta R.T. -0.129 min

Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

Tgt Ion: 97 Resp: 1078




Ion Ratio Lower Upper


97 100

99 0.0 43.1 80.1#

83 0.0 57.9 107.5#


85 0.0 38.0 70.6#

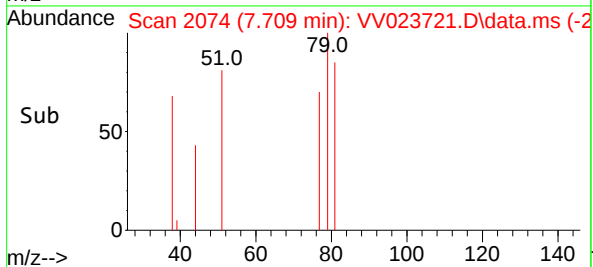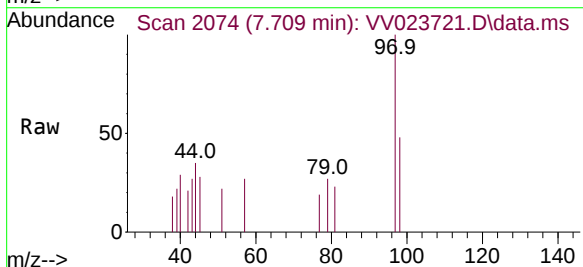






#51  
Chlorobenzene  
Concen: 0.174 ug/L  
RT: 8.882 min Scan# 2438  
Delta R.T. 0.003 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25

Instrument :  
MSVOA\_V  
ClientSampleId :







Tgt Ion:112 Resp: 4587  
Ion Ratio Lower Upper  
112 100  
114 29.2 23.3 43.3  
77 51.2 43.3 64.9



#52  
Ethylbenzene  
Concen: 2.439 ug/L  
RT: 9.011 min Scan# 2479  
Delta R.T. -0.000 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25

Tgt Ion: 91 Resp: 101480  
Ion Ratio Lower Upper  
91 100  
106 31.4 22.0 41.0




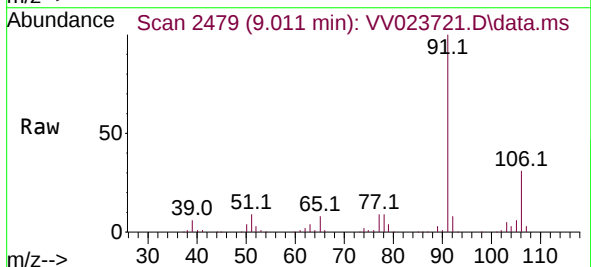


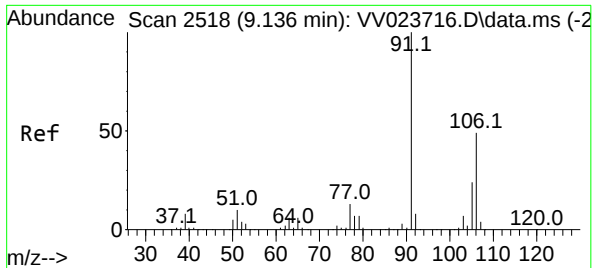

#53  
m,p-xylene  
Concen: 4.397 ug/L  
RT: 9.136 min Scan# 2518  
Delta R.T. -0.000 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25




Instrument :  
MSVOA\_V  
ClientSampleId :


Tgt Ion:106 Resp: 72806  
Ion Ratio Lower Upper  
106 100  
91 197.1 139.5 259.1

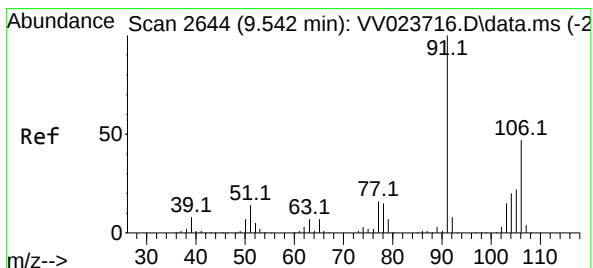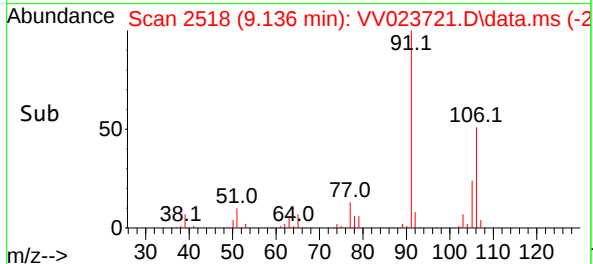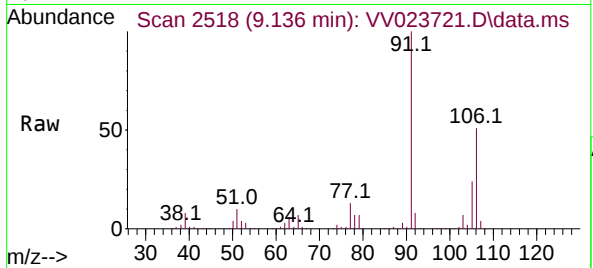

#54  
o-xylene  
Concen: 3.783 ug/L  
RT: 9.542 min Scan# 2644  
Delta R.T. -0.000 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25

Tgt Ion:106 Resp: 59575  
Ion Ratio Lower Upper  
106 100  
91 210.0 147.9 274.7


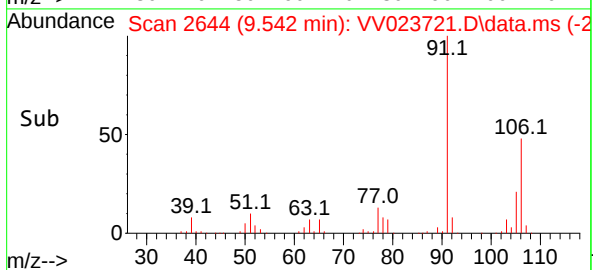

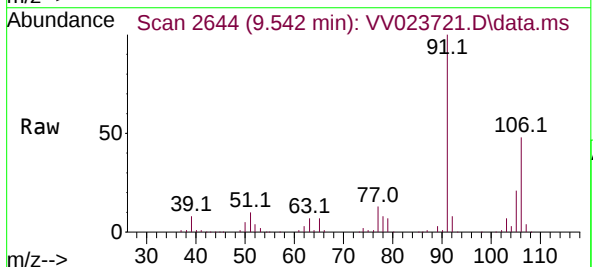




#55  
Styrene  
Concen: 0.137 ug/L  
RT: 9.542 min Scan# 21  
Delta R.T. -0.016 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25




Instrument :  
MSVOA\_V  
ClientSampleId :


Tgt Ion:104 Resp: 3627  
Ion Ratio Lower Upper  
104 100  
78 316.6 31.0 57.6#

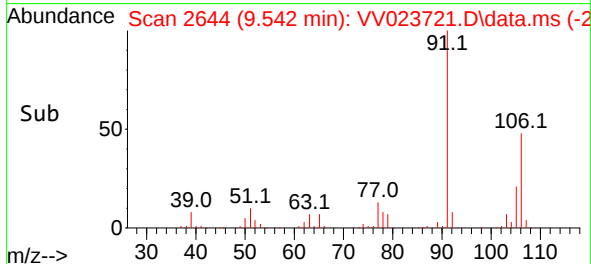

#60  
Isopropylbenzene  
Concen: 0.109 ug/L  
RT: 9.931 min Scan# 2765  
Delta R.T. -0.000 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25


Tgt Ion:105 Resp: 4435  
Ion Ratio Lower Upper  
105 100  
120 30.7 21.4 32.0  
77 20.9 12.2 18.4#

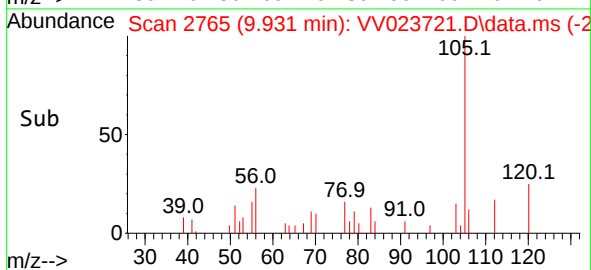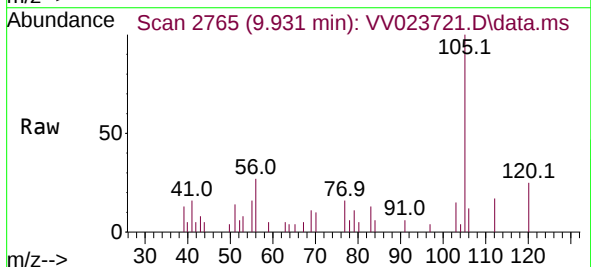






#61  
 1,2,3-Trichloropropane  
 Concen: 0.154 ug/L  
 RT: 10.014 min Scan# 21  
 Delta R.T. -0.257 min  
 Lab File: VV023721.D  
 Acq: 26 Nov 2021 13:25


Instrument :  
 MSVOA\_V  
 ClientSampleId :

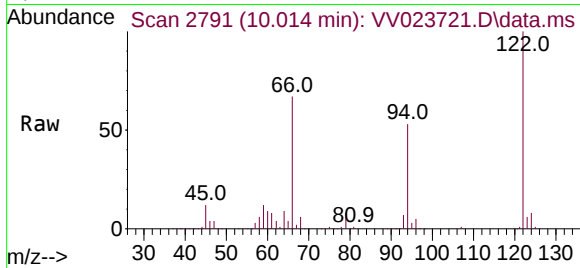



Tgt Ion: 75 Resp: 743  
 Ion Ratio Lower Upper  
 75 100  
 77 124.9 26.4 39.6#  
 110 2.7 34.2 51.2#

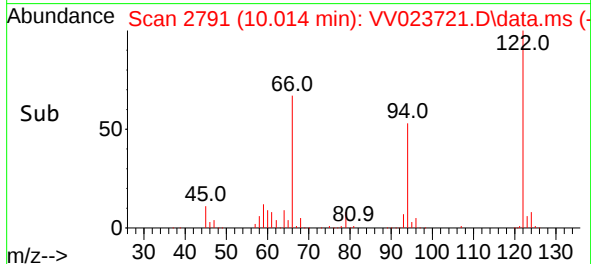


#62  
 1,3,5-Trimethylbenzene  
 Concen: 0.352 ug/L  
 RT: 10.541 min Scan# 2955  
 Delta R.T. 0.003 min  
 Lab File: VV023721.D  
 Acq: 26 Nov 2021 13:25

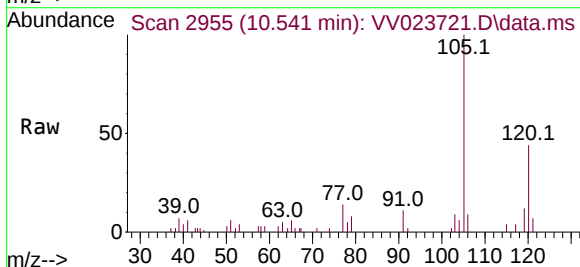

Tgt Ion: 105 Resp: 11929  
 Ion Ratio Lower Upper  
 105 100  
 120 45.7 40.1 60.1



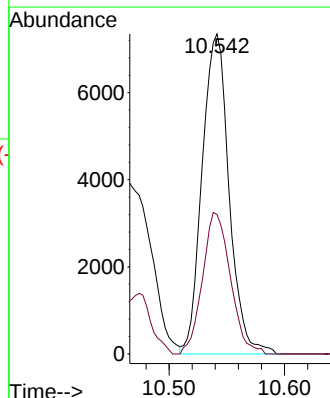





#63  
1,2,4-Trimethylbenzene  
Concen: 0.644 ug/L  
RT: 10.914 min Scan# 3070  
Delta R.T. 0.003 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25




Instrument :  
MSVOA\_V  
ClientSampleId :


Tgt Ion:105 Resp: 21568  
Ion Ratio Lower Upper  
105 100  
120 46.1 36.7 55.1

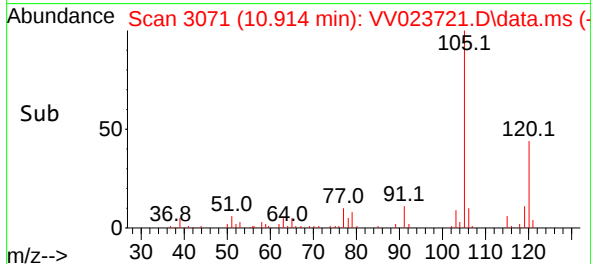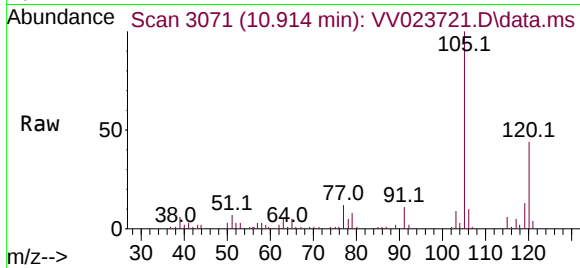

#68  
1,2-Dibromo-3-chloropropane  
Concen: 0.163 ug/L  
RT: 12.464 min Scan# 3553  
Delta R.T. 0.039 min  
Lab File: VV023721.D  
Acq: 26 Nov 2021 13:25

Tgt Ion: 75 Resp: 156  
Ion Ratio Lower Upper  
75 100  
155 0.0 71.7 107.5#  
157 0.0 103.3 154.9#

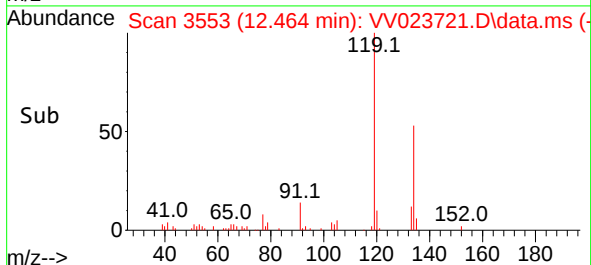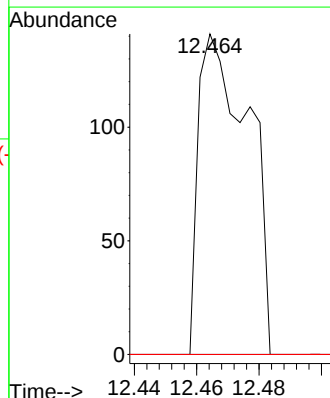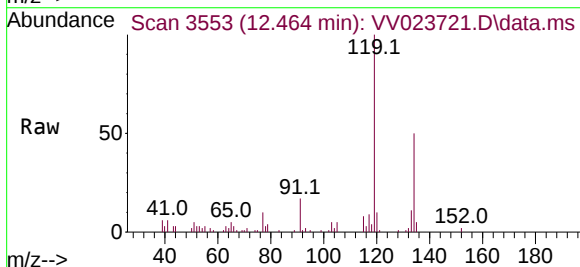



#71

Naphthalene

Concen: 3.505 ug/L

RT: 13.503 min Scan# 3876

Delta R.T. -0.000 min


Lab File: VV023721.D

Acq: 26 Nov 2021 13:25

Instrument :

MSVOA\_V

ClientSampleId :

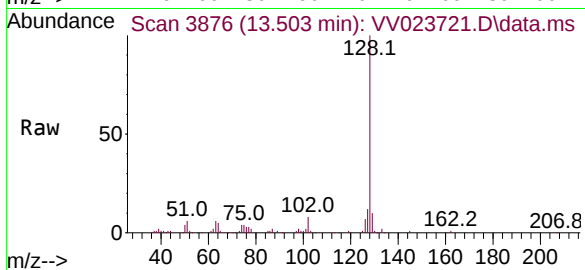

Tgt Ion:128 Resp: 59452

Ion Ratio Lower Upper

128 100

129 10.5 9.0 13.4

127 12.9 10.2 15.4

