


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023717.D
Acq On : 26 Nov 2021 11:43
Operator : SY/MD
Sample : VV1126WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Manual IntegrationsAPPROVED

Quant Time: Nov 27 03:52:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 27 03:48:32 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/29/2021
Supervised By :Mahesh Dadoda 11/29/2021

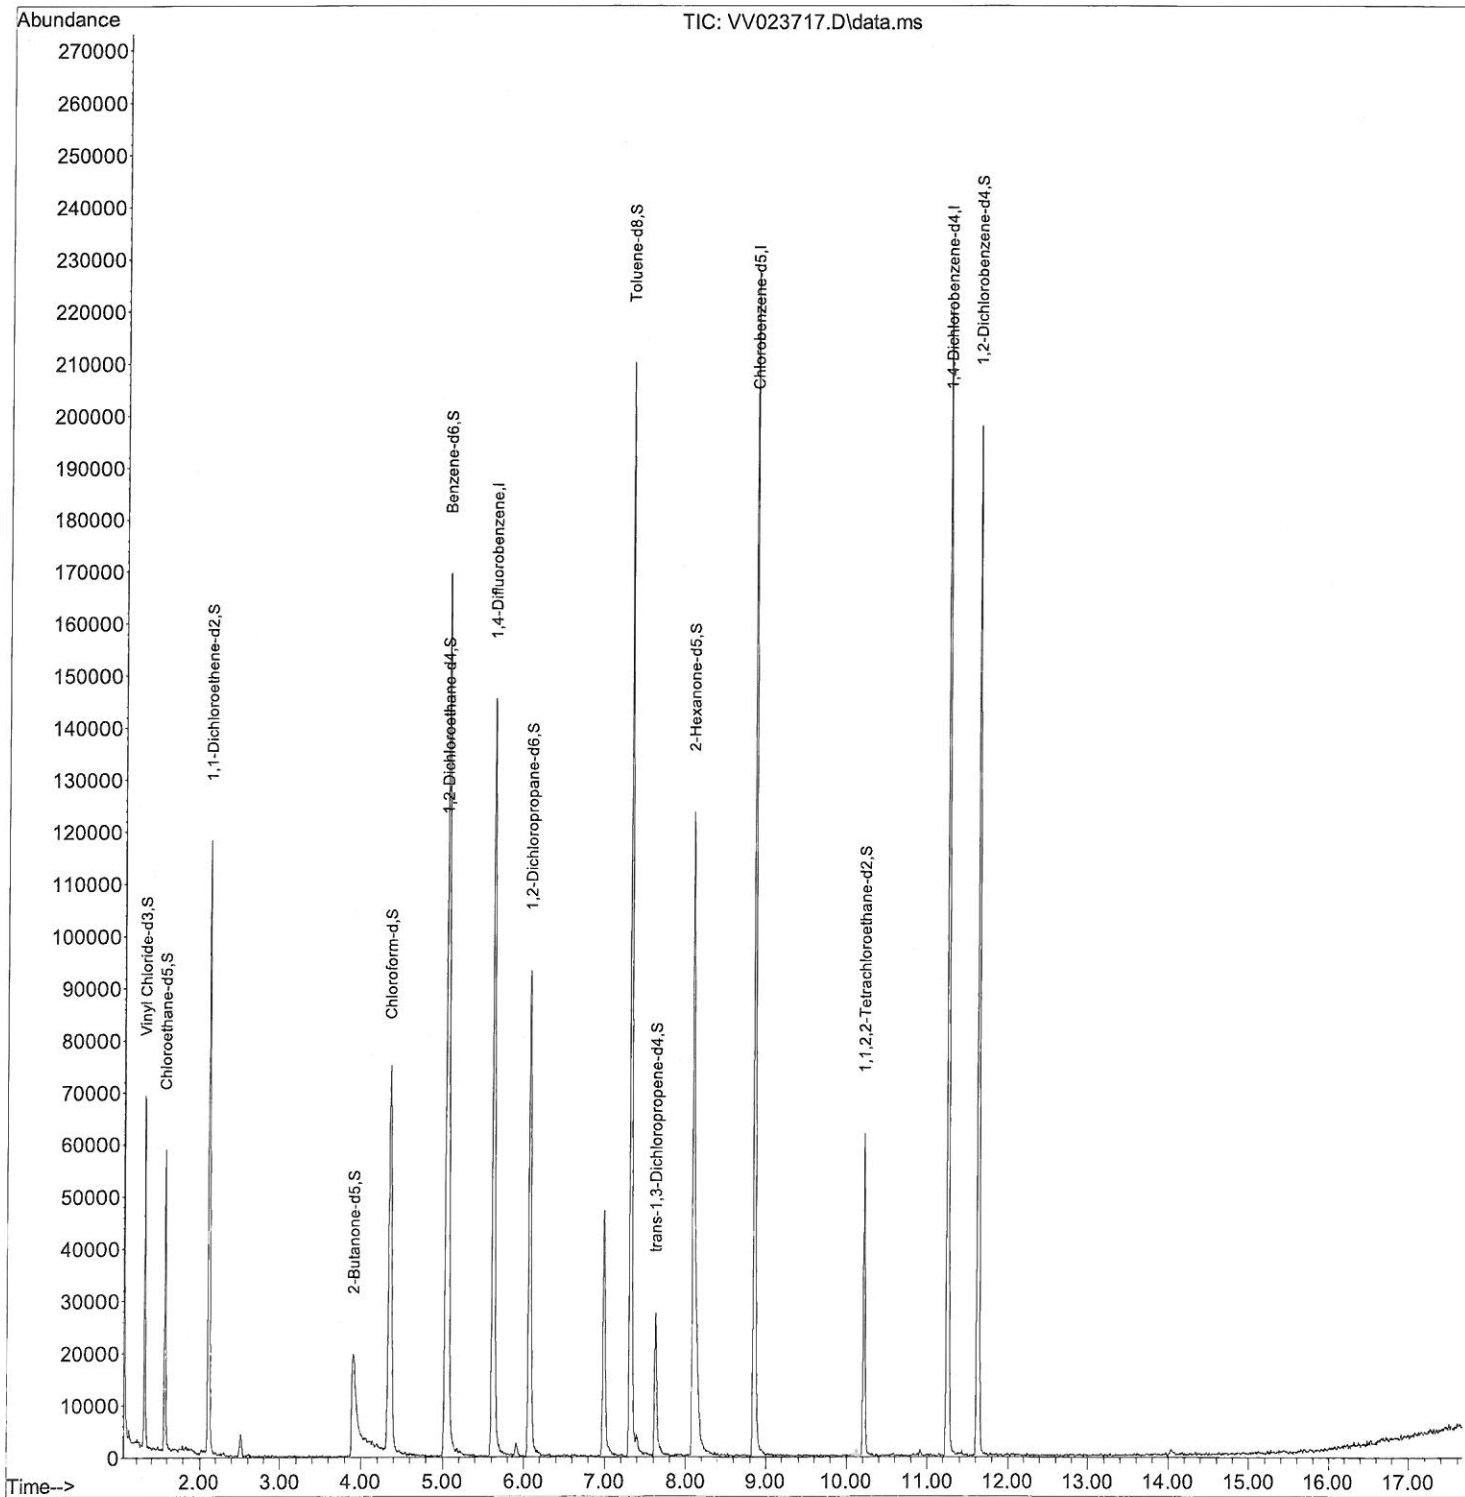




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023717.D
Acq On : 26 Nov 2021 11:43
Operator : SY/MD
Sample : VV1126WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Manual Integrations APPROVED

Quant Time: Nov 27 03:52:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 27 03:48:32 2021
Response via : Initial Calibration

Reviewed By : John Carlone 11/29/2021
Supervised By : Mahesh Dadoda 11/29/2021

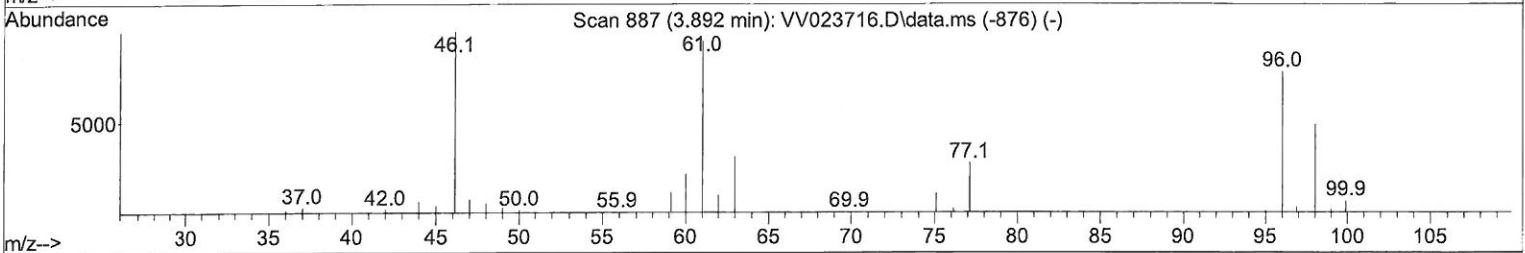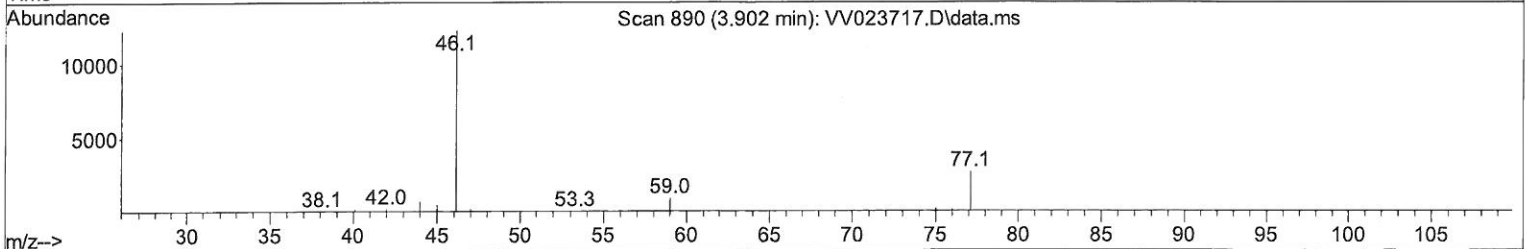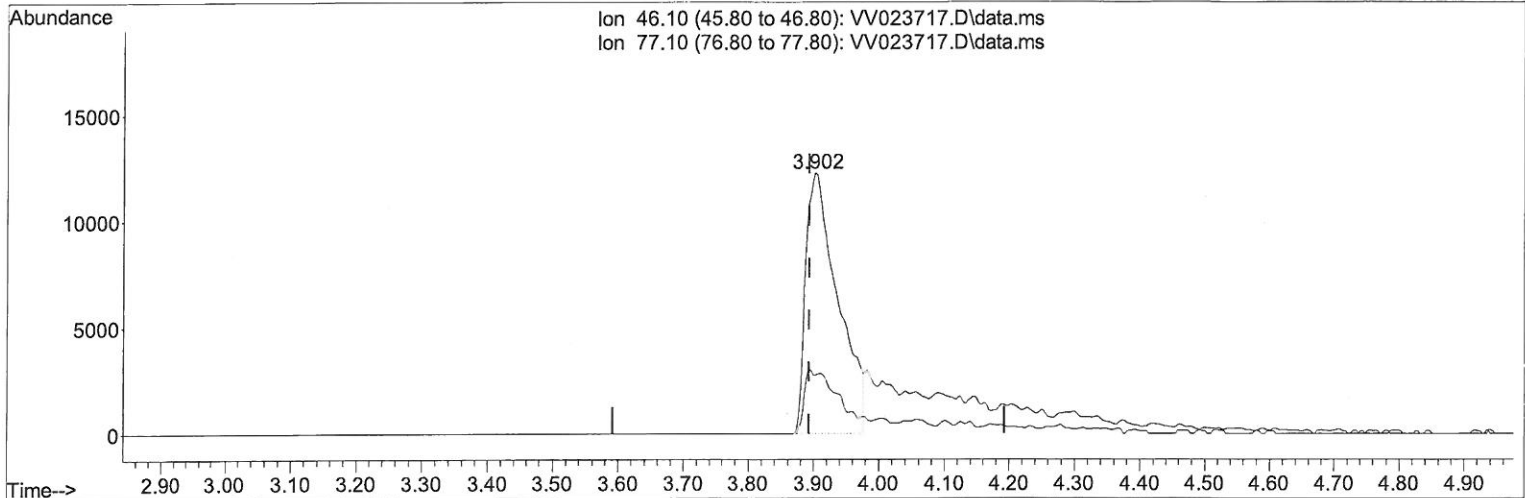

TIC: VV023717.D\data.ms

(20) 2-Butanone-d5 (S)

3.902min (+ 0.010) 33.22 ug/L

response 42261

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	8.14
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023717.D
Acq On : 26 Nov 2021 11:43
Operator : SY/MD
Sample : VV1126WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Manual IntegrationsAPPROVED

Quant Time: Nov 27 03:52:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 27 03:48:32 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/29/2021
Supervised By :Mahesh Dadoda 11/29/2021

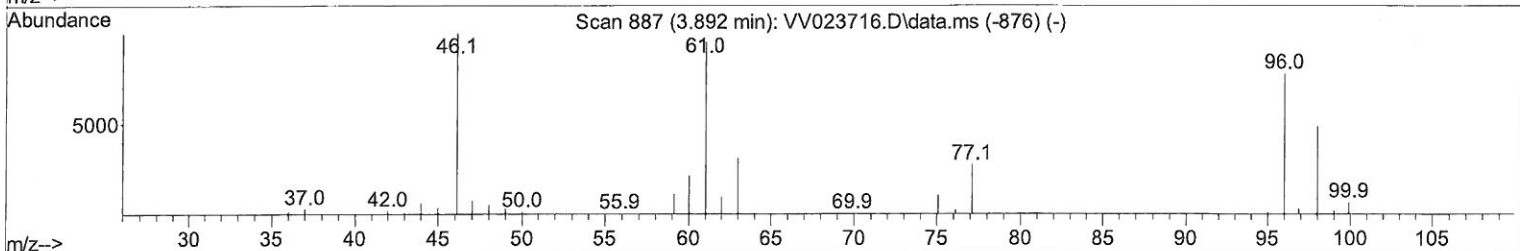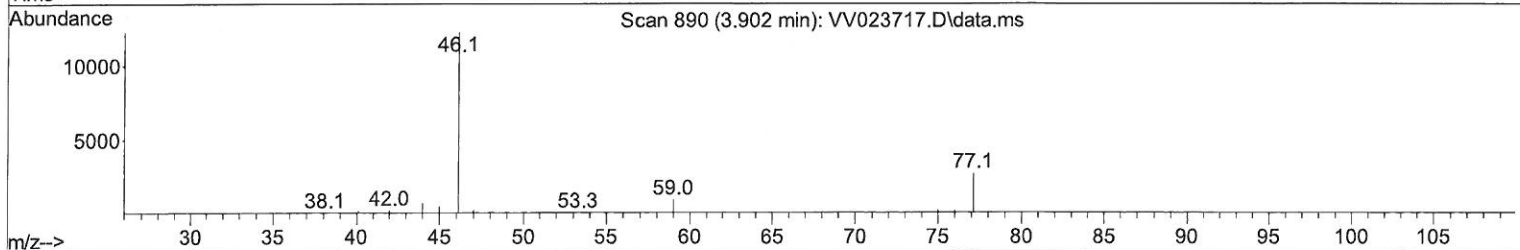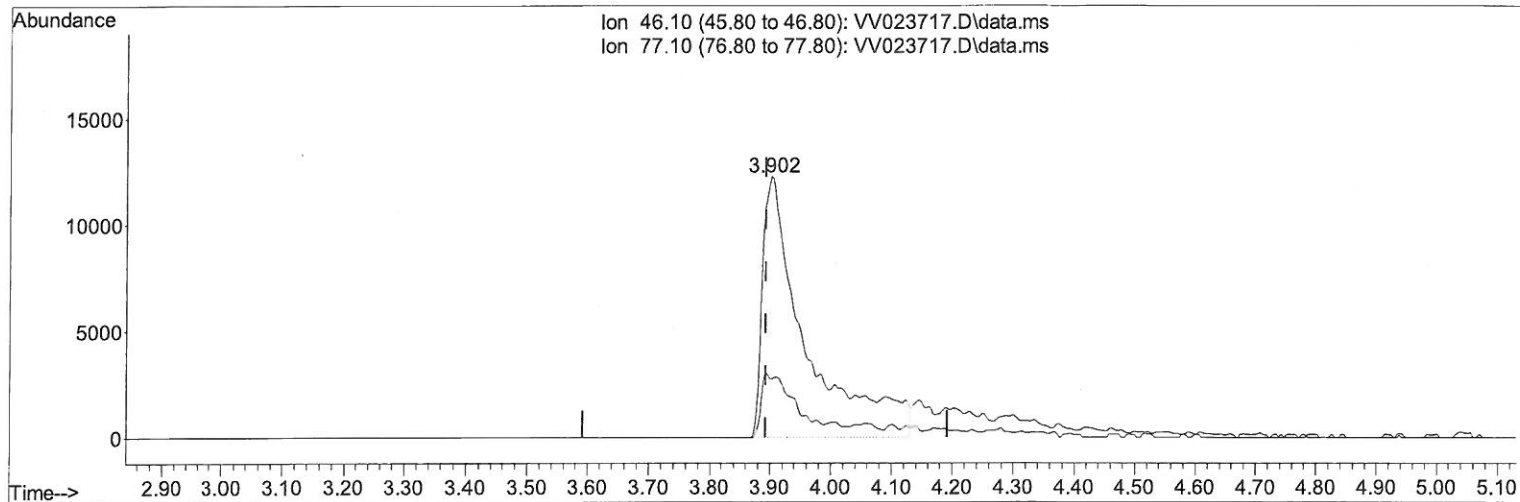

TIC: VV023717.D\data.ms

(20) 2-Butanone-d5 (S)

3.902min (+ 0.010) 47.69 ug/L m

response 60655

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	5.67#
0.00	0.00	0.00
0.00	0.00	0.00

MD
12/01/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
 Data File : VV023717.D
 Acq On : 26 Nov 2021 11:43
 Operator : SY/MD
 Sample : VV1126WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 11/29/2021
 Supervised By : Mahesh Dadoda 11/29/2021

Quant Time: Nov 27 03:52:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 27 03:48:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	128891	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	127361	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62116	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	41545	3.926	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.600%	
7) Chloroethane-d5	1.568	69	33939	4.081	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	81.600%	
11) 1,1-Dichloroethene-d2	2.108	63	60363	3.237	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.800%	
20) 2-Butanone-d5	3.902	46	60655m	47.685	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	95.380%	
24) Chloroform-d	4.346	84	74980	4.069	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	81.400%	
26) 1,2-Dichloroethane-d4	5.031	65	38416	4.463	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.200%	
32) Benzene-d6	5.047	84	157339	4.535	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
36) 1,2-Dichloropropane-d6	6.069	67	43281	4.450	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.000%	
41) Toluene-d8	7.313	98	143081	4.414	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.200%	
43) trans-1,3-Dichloroprop...	7.622	79	17403	4.439	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.800%	
46) 2-Hexanone-d5	8.088	63	54558	41.884	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.760%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29936	4.277	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	85.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	53350	4.858	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.200%	

7 MD
 12/01/21

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed