

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112621\
 Data File : VW023720.D
 Acq On : 26 Nov 2021 13:01
 Operator : SY/MD
 Sample : M4821-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4664

Quant Time: Nov 27 03:52:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 27 03:48:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	130515	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	126521	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59890	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	44512	4.155	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.000%
7) Chloroethane-d5	1.568	69	35162	4.175	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.600%
11) 1,1-Dichloroethene-d2	2.108	63	64133	3.396	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.000%
20) 2-Butanone-d5	3.895	46	72684	56.431	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.860%
24) Chloroform-d	4.349	84	82467	4.420	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	5.034	65	40098	4.601	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
32) Benzene-d6	5.053	84	165261	4.795	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
36) 1,2-Dichloropropane-d6	6.069	67	46905	4.854	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.317	98	148253	4.604	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	7.625	79	17442	4.478	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.091	63	58773	45.419	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.840%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31763	4.568	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	55980	5.287	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.800%
Target Compounds					Qvalue	
13) Acetone	2.188	43	2073	1.789	ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023720.D
Acq On : 26 Nov 2021 13:01
Operator : SY/MD
Sample : M4821-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4664

Quant Time: Nov 27 03:52:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 27 03:48:32 2021
Response via : Initial Calibration

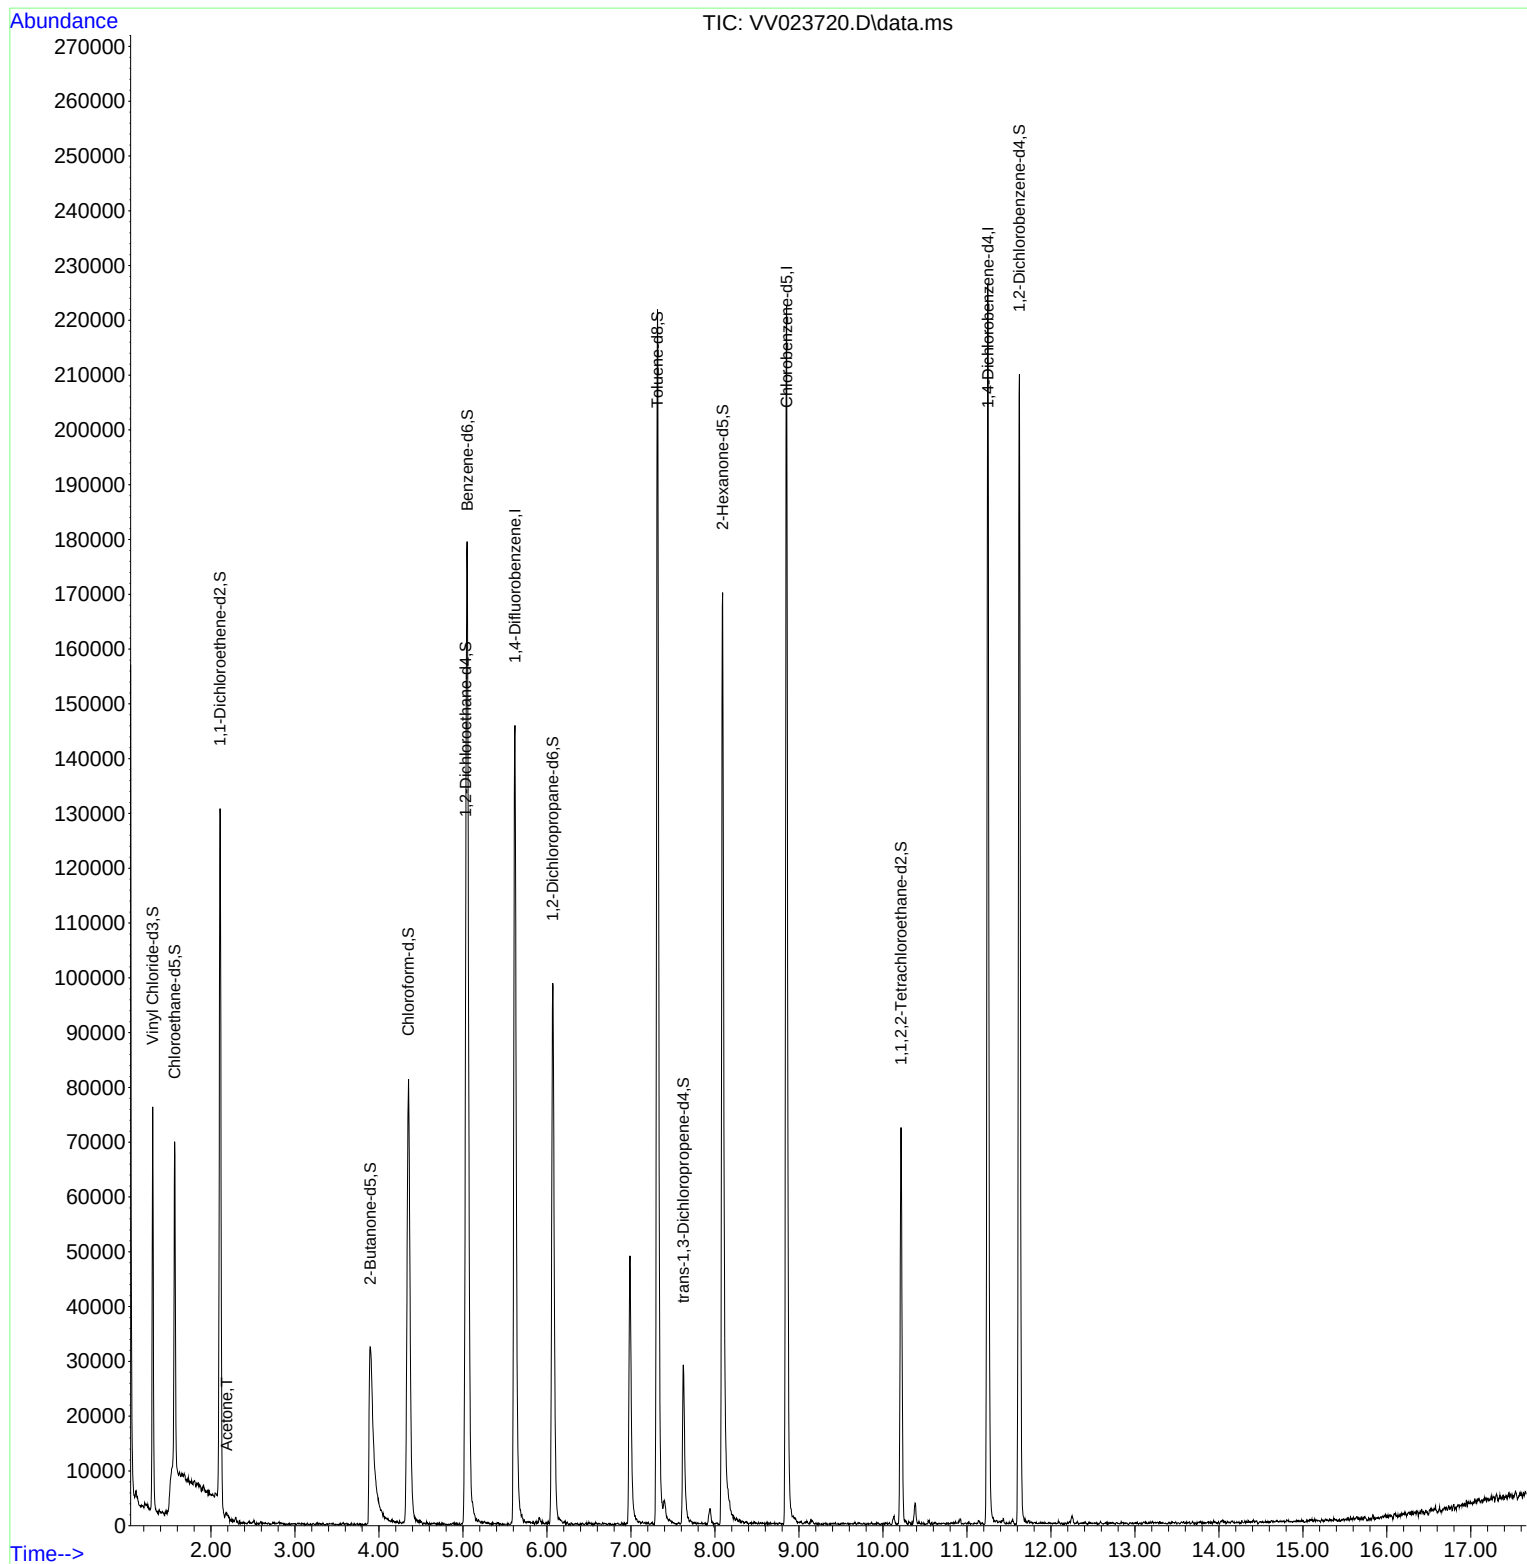

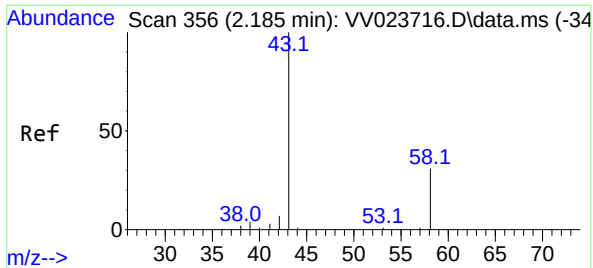

#13
 Acetone
 Concen: 1.789 ug/L
 RT: 2.188 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV023720.D
 Acq: 26 Nov 2021 13:01

Instrument :
 MSVOA_V
 ClientSampleId :
 H4664

Tgt Ion: 43 Resp: 2073
 Ion Ratio Lower Upper
 43 100
 58 9.6 0.0 41.4

