

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112621\
 Data File : VW023723.D
 Acq On : 26 Nov 2021 14:11
 Operator : SY/MD
 Sample : VIBLK242
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK242

Quant Time: Nov 27 03:53:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 27 03:48:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	132931	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	128278	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61059	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	34793	3.188	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.800%
7) Chloroethane-d5	1.568	69	31354	3.655	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.200%
11) 1,1-Dichloroethene-d2	2.108	63	48532	2.524	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.400%#
20) 2-Butanone-d5	3.892	46	83222	63.438	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.880%
24) Chloroform-d	4.349	84	76452	4.023	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.400%
26) 1,2-Dichloroethane-d4	5.034	65	39483	4.448	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%
32) Benzene-d6	5.053	84	141572	4.052	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.000%
36) 1,2-Dichloropropane-d6	6.069	67	44081	4.500	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.000%
41) Toluene-d8	7.317	98	119632	3.664	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.200%
43) trans-1,3-Dichloroprop...	7.625	79	16600	4.204	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.088	63	67369	51.349	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.700%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33511	4.754	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	52091	4.825	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.600%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	5236	0.412	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023723.D
Acq On : 26 Nov 2021 14:11
Operator : SY/MD
Sample : VIBLK242
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK242


Quant Time: Nov 27 03:53:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 27 03:48:32 2021
Response via : Initial Calibration

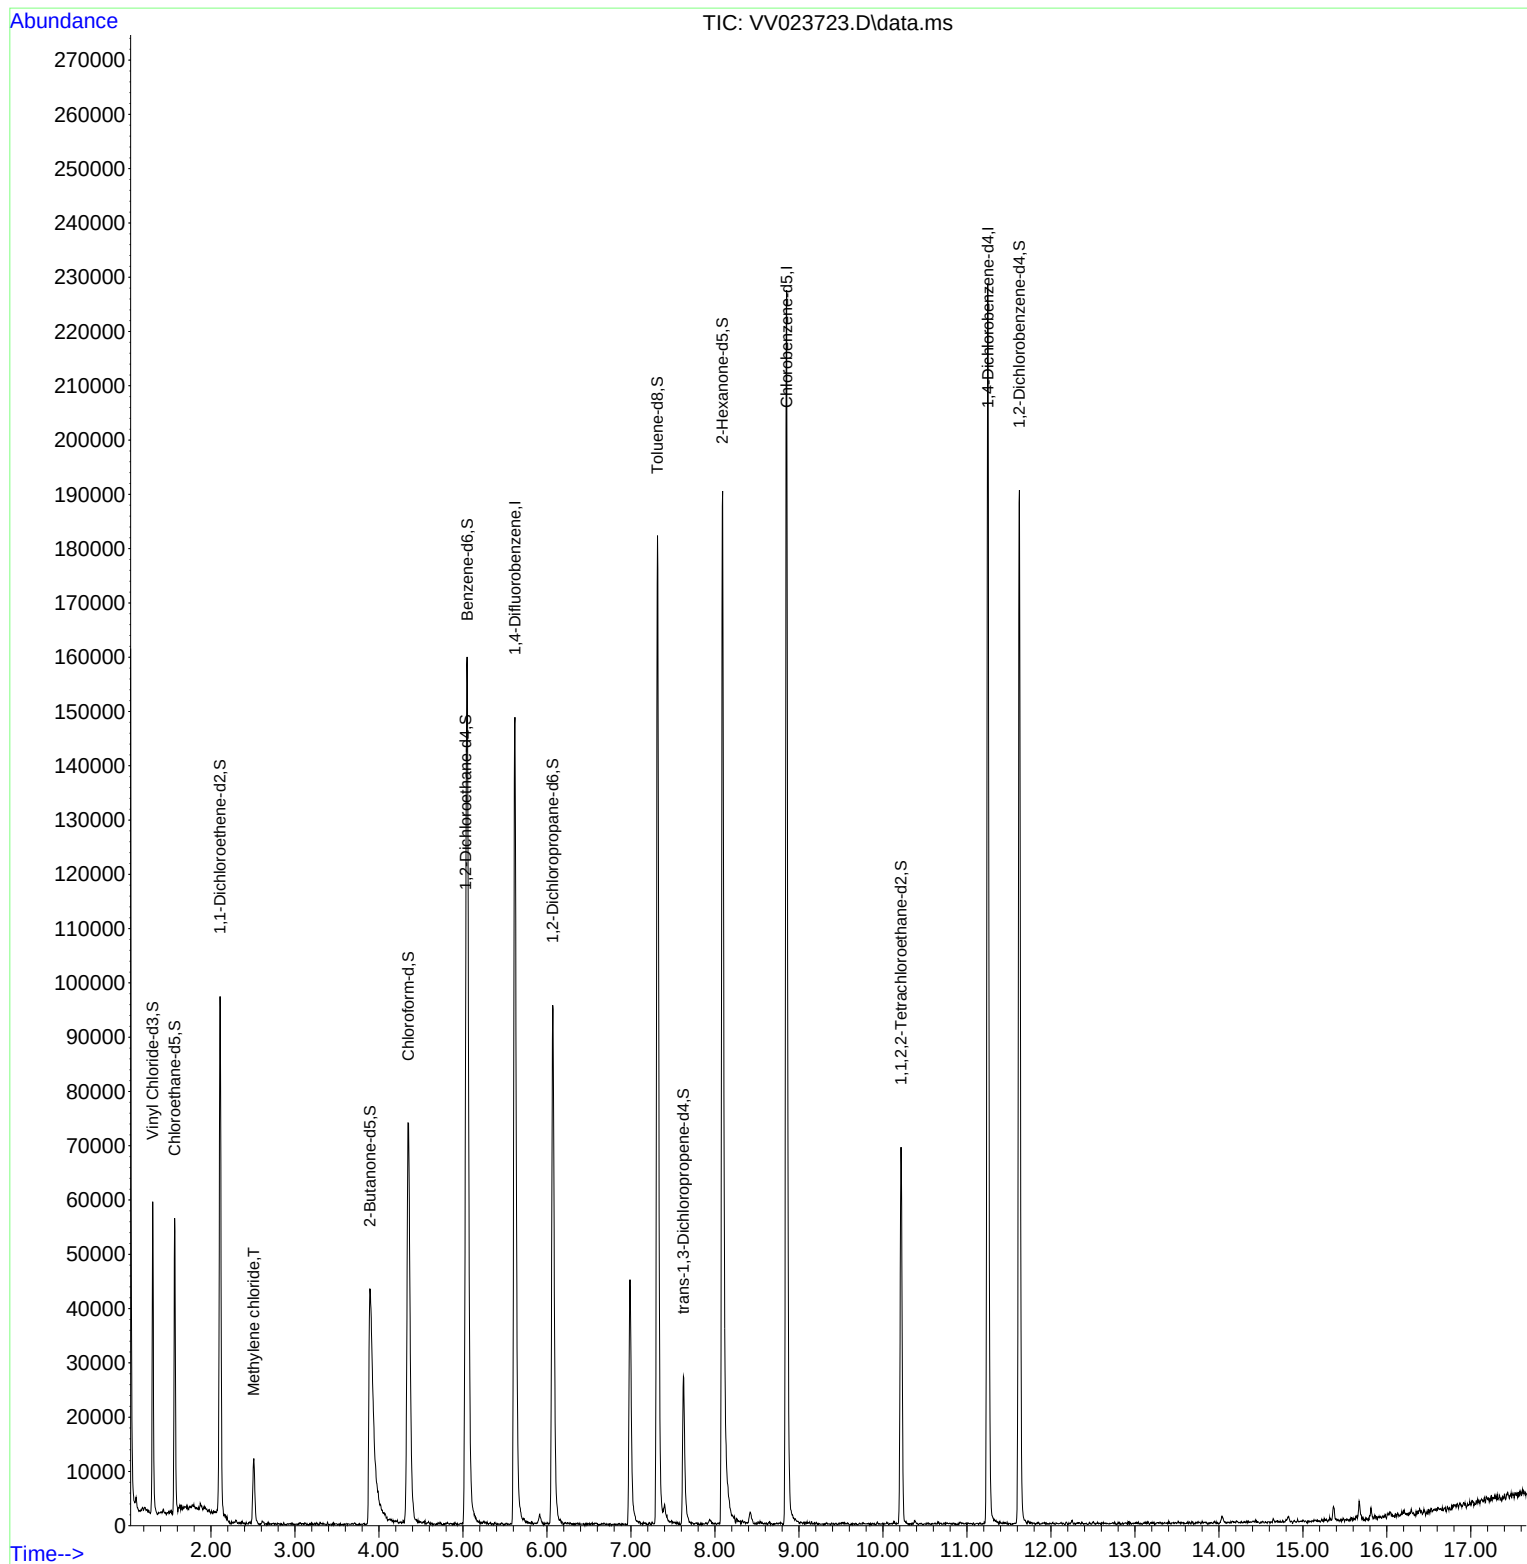

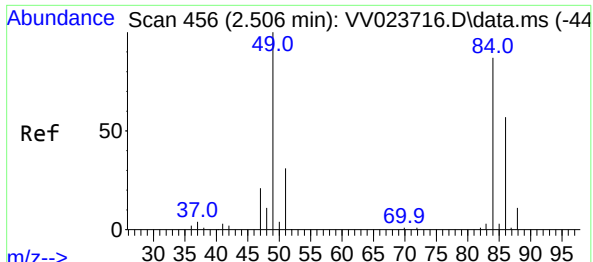

#16
Methylene chloride
Concen: 0.412 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV023723.D
Acq: 26 Nov 2021 14:11

Instrument :
MSVOA_V
ClientSampleId :
VIBLK242

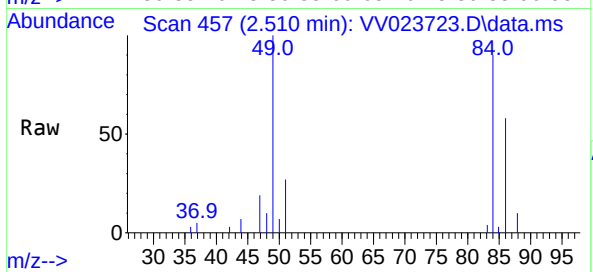

Tgt Ion: 84 Resp: 5236

Ion	Ratio	Lower	Upper
84	100		
86	64.2	42.6	79.0
49	111.0	79.7	147.9

