

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
 Data File : VV023720.D
 Acq On : 26 Nov 2021 13:01
 Operator : SY/MD
 Sample : M4821-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4664

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	73964	74989	16.65%	2.040%
2	1.568	140	164	178	rBV	67554	115137	25.56%	3.132%
3	2.108	323	332	349	rVB	129398	189563	42.08%	5.156%
4	3.895	878	888	918	rBV2	32304	116243	25.81%	3.162%
5	4.352	1012	1030	1053	rBV2	81026	202891	45.04%	5.519%
6	5.050	1229	1247	1279	rBV2	179306	450462	100.00%	12.253%
7	5.619	1412	1424	1443	rBV	145512	294541	65.39%	8.012%
8	6.069	1552	1564	1584	rBV2	98687	204744	45.45%	5.569%
9	6.989	1840	1850	1872	rBV	48892	91400	20.29%	2.486%
10	7.317	1940	1952	1971	rBV	221730	389559	86.48%	10.596%
11	7.400	1973	1978	1985	rVB6	3021	4888	1.09%	0.133%
12	7.625	2037	2048	2066	rBV	28971	53472	11.87%	1.454%
13	7.944	2135	2147	2154	rBV3	2998	5619	1.25%	0.153%
14	8.091	2182	2193	2228	rBV	170010	326800	72.55%	8.889%
15	8.853	2417	2430	2450	rBV	222441	367582	81.60%	9.999%
16	10.217	2843	2854	2866	rBV	72348	110471	24.52%	3.005%
17	10.384	2897	2906	2914	rBV3	3814	5853	1.30%	0.159%
18	11.249	3164	3175	3194	rBV	226384	339715	75.41%	9.241%
19	11.625	3281	3292	3311	rBV	209829	332410	73.79%	9.042%




Sum of corrected areas: 3676339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023720.D
Acq On : 26 Nov 2021 13:01
Operator : SY/MD
Sample : M4821-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

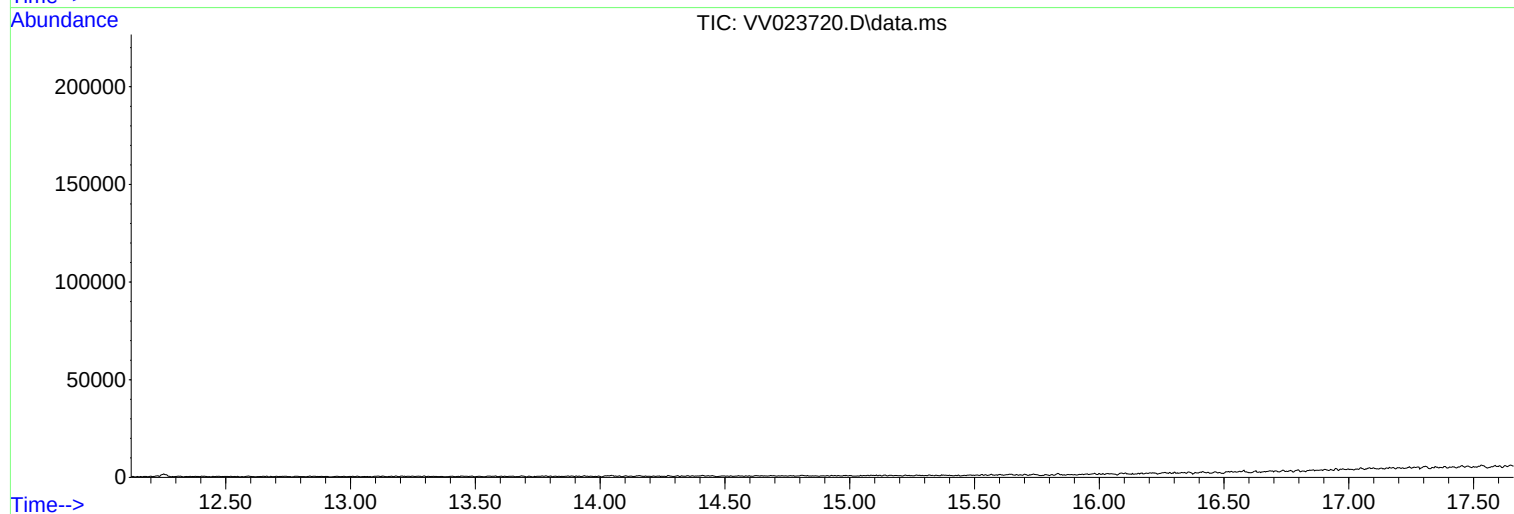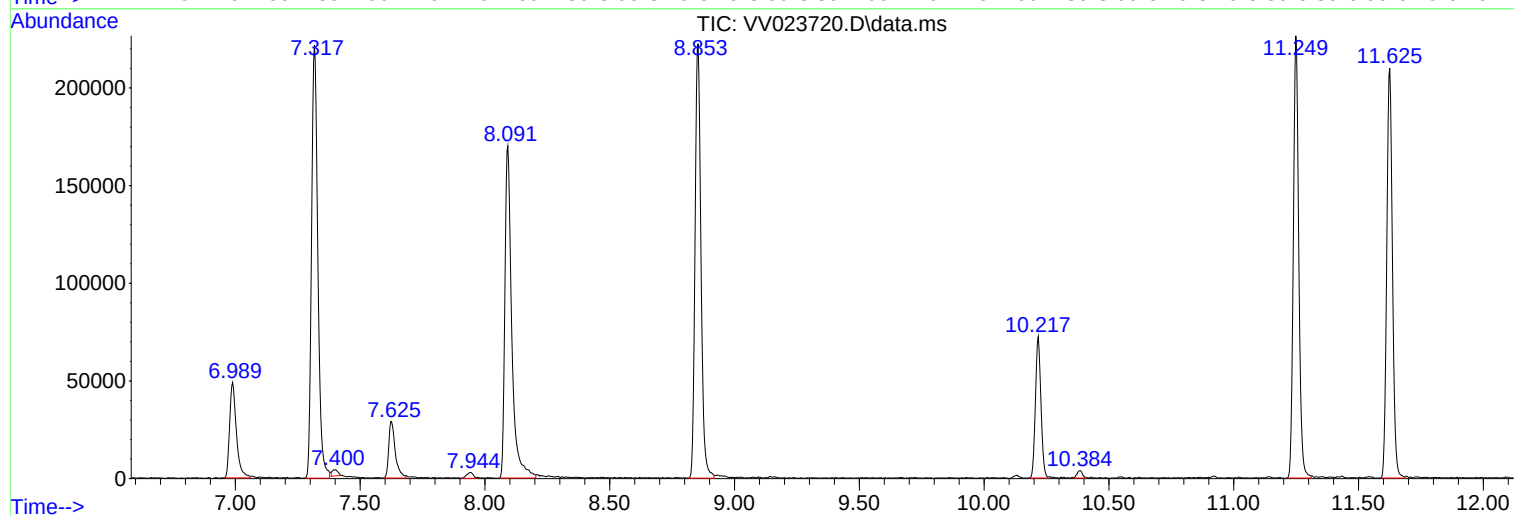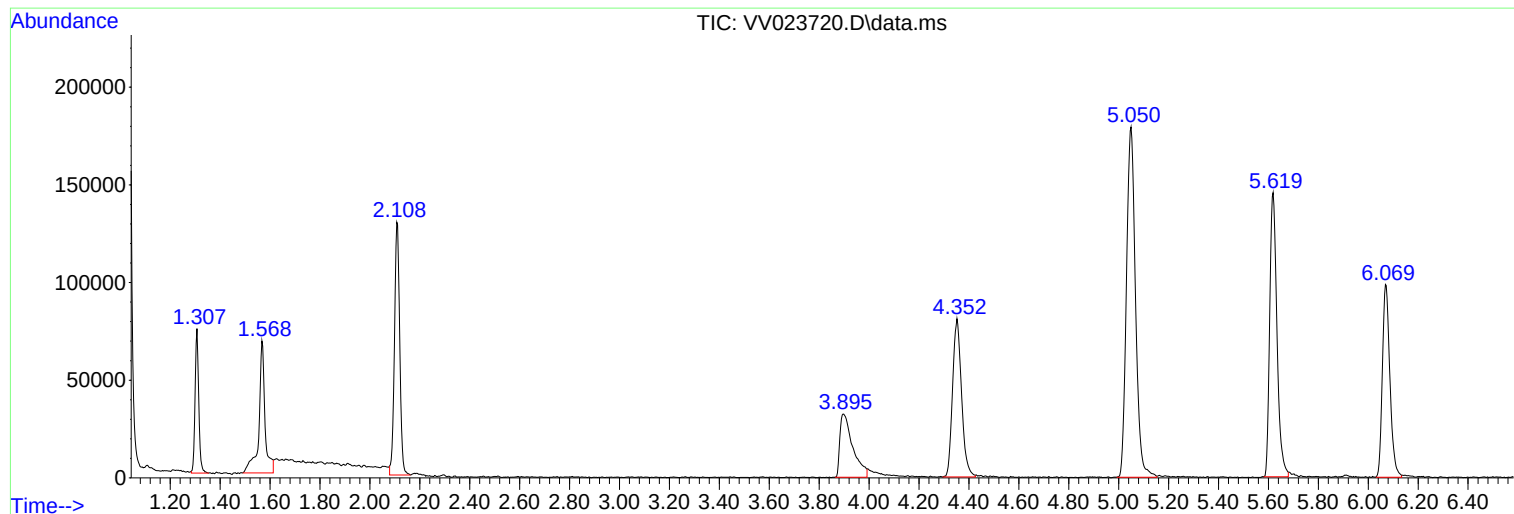

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023720.D
Acq On : 26 Nov 2021 13:01
Operator : SY/MD
Sample : M4821-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023720.D
Acq On : 26 Nov 2021 13:01
Operator : SY/MD
Sample : M4821-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc